




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷: A61B 17/02	A2	(11) International Publication Number: WO 00/15119 (43) International Publication Date: 23 March 2000 (23.03.00)
(21) International Application Number: PCT/US99/20305 (22) International Filing Date: 3 September 1999 (03.09.99) (30) Priority Data: 60/100,443 15 September 1998 (15.09.98) US (63) Related by Continuation (CON) or Continuation-in-Part (CIP) to Earlier Application US 60/100,442 (CIP) Filed on 15 September 1998 (15.09.98) (71) Applicant (for all designated States except US): MEDTRONIC, INC. [US/US]; 7000 Central Avenue NE, Minneapolis, MN 55432 (US). (72) Inventors; and (75) Inventors/Applicants (for US only): BORST, Cornelius [NL/NL]; Obrechtlaan 55, NL-3723 KB Bilthoven (NL). MANSVELT-BECK, Hendricus, J. [NL/NL]; Bildzigt 14, NL-3721 KK Bilthoven (NL). BOONE, Eric [US/US]; 7258 Walnut Avenue, Jenison, MI 49428 (US). GOODMAN, Jack [US/US]; 3228 Cottontail Court, Ann Arbor, MI 48103 (US). HALL, John, D. [US/US]; 2957 Longstreet Avenue SW, Wyoming, MI 49509 (US). O'NEILL,	William, G. [US/US]; 7267 Cuesta Way Drive, Rockford, MI 49341 (US). TESTA, Vincent, J. [US/US]; 510 North Center Drive, Grand Rapids, MI 49544 (US). VROEGOP, Eric [US/US]; 105 Birchwood, Holland, MI 49423 (US). (74) Agents: JARO, Michael, J. et al.; Medtronic, Inc. MS301, 7000 Central Avenue N.E., Minneapolis, MN 55432 (US). (81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published <i>Without international search report and to be republished upon receipt of that report.</i>	
(54) Title: METHOD AND APPARATUS FOR TEMPORARILY IMMOBILIZING A LOCAL AREA OF TISSUE (57) Abstract The invention is a method and apparatus for performing beating heart surgery, in which a single articulating arm supports multiple suction pods. Once the suction pods are applied to the heart surface, tightening a cable fixes the arm in place. Then, the suction pods may be spread apart from each other to tighten the surface of the cardiac tissue lying between the suction pods. In one embodiment, fixation of the arm as well as the spreading apart of the suction pods may occur concurrently or almost concurrently through the tensioning of a single cable. Additional embodiments of the method, system and its components are shown.		

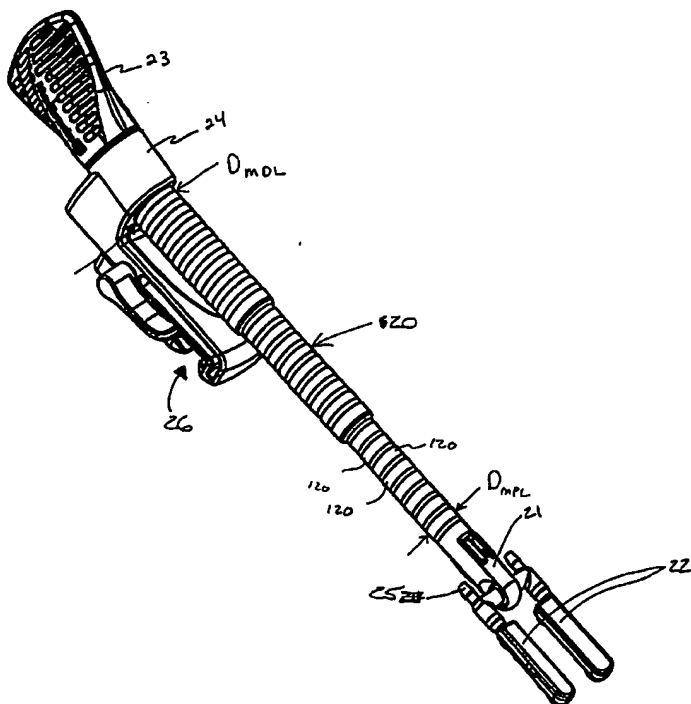

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

METHOD AND APPARATUS FOR TEMPORARILY IMMOBILIZING A LOCAL AREA OF TISSUE

FIELD OF THE INVENTION

The present invention generally relates to surgery on body tissues and organs. More specifically, the present invention relates to a method and apparatus for temporarily immobilizing a local area of tissue subject to motion, such as the heart wall, which permits a surgical procedure to be performed on that local area of tissue.

BACKGROUND OF THE INVENTION

Coronary artery disease remains the leading cause of morbidity and mortality in Western societies. Coronary artery disease is manifested in a number of ways. For example, disease of the coronary arteries can lead to insufficient blood flow to various areas of the heart. This can lead to the discomfort of angina and the risk of ischemia. In severe cases, acute blockage of coronary blood flow can result in irreversible damage to the myocardial tissue including myocardial infarction and the risk of death.

A number of approaches have been developed for treating coronary artery disease. In less severe cases, it is often sufficient to merely treat the symptoms, with pharmaceuticals, or treat the underlying causes of the disease, with lifestyle modification. In more severe cases, the coronary blockage can be treated endovascularly or percutaneously using techniques such as balloon angioplasty, atherectomy, laser ablation, stents, and the like.

In cases where these approaches have failed or are likely to fail, it is often necessary to perform a coronary artery bypass graft procedure. This procedure generally consists of the following steps: First, direct access to the heart is achieved. This is usually done by opening the chest by median

sternotomy and spreading the left and right rib cage apart; and opening the pericardial sac to achieve direct access to the heart.

Next, a blood vessel or vessels for use in the graft procedure are mobilized from the patient. This usually entails mobilizing either a mammary artery or a saphenous vein, although other graft vessels may also be used.

Next, a heart-lung or cardiopulmonary bypass is performed. This usually entails arterial and venous cannulation, connecting the bloodstream to a heart-lung machine, cooling the body to about 32 degrees Celsius, cross-clamping of the aorta and cardioplegic perfusion of the coronary arteries to arrest and cool the heart to about 4 degrees Celsius. The arrest or stoppage of the heart is generally required because the constant pumping motion of the beating heart would make surgery upon the heart difficult in some locations and extremely difficult if not impossible in other locations.

Once cardiac arrest is achieved, then a graft (or grafts) is attached to the relevant portions of a coronary artery (or arteries) followed by weaning from the cardiopulmonary bypass, restarting the heart and decannulation. Finally the chest is closed.

One area which may create difficulties for the patient and extra expense and time for the procedure involves the cardiopulmonary bypass. In a cardiopulmonary bypass all the patient's blood, which normally returns to the right atrium, is diverted to a system which supplies oxygen to the blood and removes carbon dioxide and returns the blood, at sufficient pressure, into the patient's aorta for further distribution into the body. Generally such a system requires several separate components, including an oxygenator, several pumps, a reservoir, a blood temperature control system, filters as well as flow, pressure and temperature sensors.

Problems may develop during cardiopulmonary bypass due to the reaction blood has to non-endothelially lined surfaces, i.e. surfaces unlike those of a blood vessel. In particular, exposure of

blood to foreign surfaces results in the activation of virtually all the humoral and cellular components of the inflammatory response, as well as some of the slower reacting specific immune responses. Other complications from cardiopulmonary bypass include loss of red blood cells and platelets due to shear stress damage. In addition, cardiopulmonary bypass requires the use of an anticoagulant, such as heparin. This may, in turn, increase the risk of hemorrhage. Finally cardiopulmonary bypass sometimes necessitates giving additional blood to the patient. The additional blood, if from a source other than the patient, may expose the patient to blood born diseases.

Due to the risks incurred during cardiopulmonary bypass, others have attempted to perform a coronary artery bypass graft procedure without cardiac arrest and cardiopulmonary bypass. For example, Trapp and Bisarya in "Placement of Coronary Artery Bypass Graft Without Pump Oxygenator", *Annals Thorac. Surg.* Vol. 19, No. 1, (Jan. 1975) pgs. 1-9, immobilized the area of the bypass graft by encircling sutures deep enough to incorporate enough muscle to suspend an area of the heart and prevent damage to the coronary artery. More recently Fanning et al. in "Reoperative Coronary Artery Bypass Grafting Without Cardiopulmonary Bypass", *Annals Thorac. Surg.* Vol. 55, (Feb. 1993) pgs. 486-489 also reported immobilizing the area of the bypass graft with stabilization sutures.

Current beating heart bypass surgery techniques demand relatively motionless epicardial tissue in the immediate vicinity of an anastomosis. Several systems are presently available which attempt to immobilize epicardial tissue in the immediate vicinity of an anastomosis through a simple mechanical fork. One of the many such systems presently available includes the Access™ system available from CardioThoracic Systems Inc., Cupertino, California. Such a system stabilizes the heart by pressing a fork downwards onto the heart surface. Through this pressure the region of the epicardium between the fork is immobilized. Commercially available systems use short arms mounted to retractors in close

proximity to the chest cavity. Mechanical fork systems only operate successfully on vessels that can be immobilized by applying pressure in a downward direction. These systems are very useful for operations on the anterior portion of the heart (such as the left anterior descending artery). However, fork systems are limited in their ability to maneuver a vessel into better view or for operating on the posterior portion of the heart. That is, fork systems are limited in their ability to "present" a vessel to the surgeon. This is a even greater drawback since fork systems stabilize only through compression, therefore often pushing downwards the are of surgical interest. In addition, compression of the heart can lead to diminished cardiac output, presenting a further risk to the patient's well-being. Finally, such systems, to date, have often featured rigid, inflexible arms which often interfere with the view or movements or both of the surgeon.

Suction stabilization systems, such as the Medtronic Octopus® Tissue Stabilizer and Accessories (available from Medtronic, Inc., Minneapolis, Minnesota USA), use comparatively long, dual reusable articulating arms configured with clamps at their distal ends to secure suction based tissue stabilizers. During use, the arms are typically secured to a rail on the side of the operating table. The suction grips and immobilizes the surface of the heart. Additionally, the system allows the surgeon to manipulate the anastomosis site into better view by rotating and supporting the heart. The system also allows the surgeon to apply tension to the tissue between the stabilizers. Thus, the system is much more versatile than mechanical fork style systems. The suction paddles or pods can attach to and immobilize the heart, and can be used to manipulate the heart into better position so that the more difficult to reach vessels can be bypassed.

Many surgeons have used the Medtronic Octopus® Tissue Stabilizer system to perform as many as five or six vessel bypasses. Some surgeons, in fact, report using the product on 50-90% of their cases. Nonetheless such a system is still in need of improvement. For example, such a system

was relatively more cumbersome to set up than desired, requiring each stabilization arm to be individually fixed or immobilized. Moreover, because each arm worked individually, spreading the arms relatively apart was more difficult than desired. Finally, because the degree of spreading was not limited in any way, surgeons could spread the paddles apart at greater distance than desired, causing one or both paddles to spontaneously lose capture of the tissue.

While these past products and attempts have achieved some success, there still exists a need to provide a method and apparatus for performing beating heart surgery which readily and quickly permits the immobilization or stabilization of a local area of tissue.

The present invention concerns an advanced system for immobilizing or stabilizing a local area of tissue.

SUMMARY OF THE INVENTION

The invention is a method and apparatus for performing beating heart surgery, in which a single articulating arm supports multiple suction paddles or pods. Once the suction pods are applied to the heart surface, tightening a cable fixes the arm in place. Then, the suction pods may be spread apart from each other to tighten the surface of the cardiac tissue lying between the suction pods. In one embodiment, fixation of the arm as well as the spreading apart of the suction pods may occur concurrently or almost concurrently through the tensioning of a single cable. Additional embodiments of the method, system and its components are shown.

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other aspects of the present invention will best be appreciated with reference to the detailed description of the invention in conjunction with the accompanying drawings, wherein:

FIGS. 1-1 through 1-4 show various views of a preferred embodiment of the invention.

FIG. 2 is an alternate embodiment of the present invention.

FIG. 3 is an exploded perspective view of the cable tensioning and device clamping mechanisms.

FIG. 4 is a perspective view of the first of three preferred embodiments for tightening/spreading mechanism 21.

FIG. 5 is an exploded perspective view of the tightening components of **FIG. 4**.

FIG. 6 is a perspective view of the second of three preferred embodiments for tightening/spreading mechanism 21.

FIG. 7 is an exploded perspective view of the tightening components of **FIG. 6**.

FIG. 8 is a perspective view of the third of three preferred embodiments for tightening/spreading mechanism 21.

FIG. 9 is an exploded perspective view of the tightening components of **FIG. 8**.

FIGS. 10-40 show additional features and alternative embodiments of the present invention.

The **FIGS.** are not necessarily to scale.

DETAILED DESCRIPTION OF THE PRESENT INVNETION

The present invention is a method and apparatus for performing beating heart surgery, in which a single articulating arm supports multiple suction pods. Once the suction pods are applied to the heart surface, tightening a cable fixes the arm in place. Then, the suction pods may be spread apart from each other to tighten the surface of the cardiac tissue lying between the suction pods. In one embodiment, fixation of the arm as well as the spreading apart of the suction pods may occur concurrently or almost concurrently the tensioning of a single cable. Additional embodiments of the system and its

components are shown. Support for conventional aspects of the invention may be found in the enclosed documents, all of which are incorporated by reference in their entirety.

US 5,727,569 (Benetti *et al.*)

WO 95/01757 (Borst)

US 5,782,746 (Wright)

WO 97/10753 (Borst *et al.*)

Preferred embodiments of the invention are shown in the enclosed FIGS., and are described in detail

below.

FIG. 1-1 is a perspective view of a preferred embodiment of the invention. An articulating arm 20 is attached to support 24 on the proximal end of the arm, and terminates with tightening/spreading mechanism 21 at the distal end of the arm. On the opposite, more proximal, end of support 24 is handle 23. Distally beyond tightening/spreading mechanism 21 is a plurality (as shown, two) of suction paddles or pods 22. Each suction pod 22 can be connected to vacuum by a conventional connection 25 that lies at the proximal end of pod 22. Each pod and its suction ports may be constructed in any acceptable manner, such as the same as that used in the Medtronic Octopus™ tissue stabilizer. Clamp 26 lies below support 24 and is designed to attach the entire device to conventional surgical retractors and other similar equipment (not shown). The preferred embodiment shown in **FIG. 1-1** is illustrative but not intended to be limiting insofar as the scope of the invention is concerned. For example, the handle 23 is shown in a preferred and highly stylized embodiment, but any device which performs the functions of the handle as described below would suffice.

Articulating arm 20 comprises a plurality of "ball and socket" links. **FIG. 1-2** is a cross sectional view of a link used in the arm of the present invention. As seen, each link 120 has a hole 123 that passes through its center. Each link 120 comprises, on its distal end, a hemispherical protrusion 121; and on its proximal end, a hemispherical indentation 122. The hemispherical shapes of adjacent links are nearly identical, such that the links rotate smoothly against one another provided they are not under undue tension with each other.

Turning now to **FIG. 1-3** which is a partial view of a section of the links and cable showing the engagement of the cable with the side wall of the links as the arm is bent. A cable 40 passes through hole of all of the links and is connected between the handle 23 and the tightening/spreading mechanism 21. Rotation of handle 23 tightens the cable and causes the links to hold against each other in place. Immobilization of the links relative to each other during tightening of the cable is facilitated by the shape of the hole 123. As seen, hole is flared, having a larger opening with the surface of the hemispherical protrusion 121 and a smaller opening through the surface of the hemispherical indentation 122. The links, as seen in **FIG. 1-1**, vary in size along the length of the arm, with the links in the most proximal portion of the arm being largest, the links in the most proximal portion the smallest and the middle portion somewhere in between. In the preferred embodiment the links have the following outer diameters and radius of curvature for the hemispherical protrusion and radius of curvature for the hemispherical indentation along each of these portions as follows:

Portion of arm	R ₁ (inches)	R ₂ (inches)	DIA(inches)
Most distal portion	0.251	0.250	0.514
Middle portion	0.313	0.311	0.637
Most proximal portion	0.317	0.374	0.763

In the preferred embodiment, the links are fabricated out of highly rigid engineered thermoplastics such as glass filled Ultem™ (available from GE Plastics, Pittsfield, Massachusetts.) Preferably the highly rigid engineered thermoplastics includes at least 20% glass fiber, and better still at least 30% glass fiber. This material offers stiffness comparable to metal systems, and yet can be manufactured at costs that allow for single use disposability. The cable is preferably a multi-stranded stainless steel cable having between approximately 7 to 19 strands. The links and cable may also be manufactured from other materials, including any other suitable highly engineered polymers including

any number of available liquid crystal polymers for the links, as well as many other types of cables, including bundle stranded, braided or cabled titanium as well as Kevlar™ for the cable.

The preferred embodiment also employs a textured surface molded or otherwise formed into the hemispherical features of the links. When the links are pulled together during tightening, the texturing causes an increase in coefficient of friction between the adjacent spherical surfaces. This has the highly-desirable benefit of increasing overall system stiffness. This is depicted in FIG. 1-4, which depicts the roughened surfaces between the ball and socket, such that in tension, the elements are more securely linked together. As seen, in the preferred embodiment, the texture provided is irregular, that is, the texture is non-uniform, and has an average height spanning approximately (peak to valley) of between 20 to 100 microns, with an average height ($height_{avg}$) spanning approximately 40 microns preferred. As seen in FIG. 1-5, moreover, in an alternative embodiment texture may be provided through a symmetrical structure, depicted here as a series of interlocking dimples 127 and hemispheres 128. Other geometries may also be used, including both surface having the same elements, such as hemispheres, as well as other shapes, including notches or grooves, to name only a few.

In this embodiment, articulating arm links 120 have a decreasing outer diameter from the proximal portion to distal end portion of the arm. This is also seen in FIG. 1-1, where outer diameter of the most proximal link portion D_{MPL} is larger than that of the outer diameter of the middle link portion D_{MLP} which, in turn, is larger than that of the outer diameter of the most distal link portion D_{MDL} . Decreasing the link diameter allows a lower profile assembly that improves the ability of the surgeon to use the device without unduly restricting accessibility to the surgical site while further ensuring adequate rigidity. In the preferred embodiment D_{MPL} is approximately 0.75 inches, D_{MDL} is approximately 0.50 inches and the D_{MLP} a outer diameter of approximately 0.625 inches, and the total arm length is approximately 10.25 inches with the pods and approximately 9 inches without the pods.

Further, in the preferred embodiment most proximal link portion features 19 links, middle link portion features 4 links, and most distal link portion features 3 links.

In an alternate embodiment, as shown in **FIG. 2**, the links of articulating arm 20 are covered with a thin walled elastomeric sheath 27. The sheath serves to prevent fragile sutures from catching on the edges where the links join. Sheath is preferably manufactured of silicone rubber, although other materials, such as latex rubber or polyurethane or even collagen, may also be used.

FIG. 3 is an exploded perspective view of the cable tensioning and device clamping mechanisms. Tension is applied to cable 40 by a torque screw and nut configuration at the proximal end of the device. Cable 40 passes through mount 24, and then through the bore of torque screw 25, and terminates in a swaged connector 27. In the preferred embodiment shown, the torque screw interacts with a corresponding nut portion 13 which is integrally formed within handle 23, although an embodiment in which handle 23 turned a separate nut is within the scope of the invention. Torque screw preferably is threaded at 12 threads per inch. As handle 23 is rotated, torque screw 25 engages nut portion 13 and advances proximally into handle 23, tensioning cable 40. It is preferred, for safety purposes, for the degree or amount of cable tensioning in the system to be limited. In the preferred embodiment this is accomplished by sizing housing 24, torque screw 25, and handle 23 such that torque screw 25 may advance into handle 23 along nut portion only a predetermined amount. In such a manner the system is configured so that the cable may not be over-tensioned, i.e., tightening of cable 40 is limited so as to remain comfortably below the rated strength of cable 40.

The torque screw, through the mechanical advantage of a 12 thread per inch torque screw allows cable tensions as high as 500 lb. to be applied by hand. While the actuation is somewhat slower than possible other type actuators (e.g. scissors-type actuator) the high tension in the cable optimizes arm rigidity.

Arm rigidity is further enhanced through the interplay between the multi-stranded cable riding on the inner diameter of the plastic segments. The multi-stranded cable riding on the inner diameter of the plastic segments induces additional friction which optimizes stability. As the cable is tensioned at high load values (>200 lb.), the cable digs into the inner diameter of the softer plastic of the segments. This is depicted above in regards to FIG. 1-3 which is a partial view of a section of the links and cable showing the engagement of the cable with the side wall of the links as the arm is bent. Since the cable is striated with typically 7-19 strands, the result is a strong interlocking of cable and plastic segments. The interlocking of the stranded cable to the plastic segment increases the coefficient of friction between cable and plastic segment. This further locks up segments to each other since they cannot slide easily along the cable. Thus enhancing arm rigidity. Below sufficient cable tension, however, the cable does not dig into the links and cause the strong increase in coefficient of friction. Additional embodiments of the invention may also feature cables of greater surface roughness, as well as sheathing the cable in materials sheaths having a greater coefficient of friction than the cable itself. Such friction enhance sheaths are particularly believed useful where cables other than stranded cables are used, such as Kevlar™ cables, as mentioned above.

The complete device is designed to be clamped to a wide variety of commonly used sternal retractors. Clamping mechanism 26 comprises mating portions of mount 24 and a movable jaw 28, each configured to provide half of a dovetail shaped groove. Movable jaw 28 is attached to mount 24 by a center pin 29 that passes through a groove 28 in the movable jaw 28. Center pin 29 also passes through conical spring washer 30. Groove 35 allows movable jaw 28 slide back and forth, permitting mounting to retractor elements of varying width. Center pin 29 comprises a cross hole 31. A Cam pin 36, which is rigidly affixed to a knob 33, passes through cross hole 31, capturing together the movable jaw 28 and the mount 24. Cam pin 36 has an off-axis lobe 32 which induces upward movement on

center pin 29 when knob 33 is advanced forward (in the FIG. 3, clockwise) to a horizontal position parallel to the cable 40. This upward motion compresses spring washer 30, which pulls the two halves of the clamp together. This induces, onto the retractor, both horizontal and vertical clamping forces in the dovetail features of the clamp halves, securing the clamp in place. Movable jaw 28 is additionally provided with dual compression springs 34 which bias the clamp to a fully forward position. This provides more convenient mounting of the clamp, and also ensures a more reliable connection between the mount and retractor element.

FIG. 4 is a perspective view of the first of three preferred embodiments for tightening/spreading mechanism 21. FIG. 5 is an exploded perspective view of the tightening components of FIG. 4. The embodiment of FIGS. 4 and 5 provides simultaneous parallel translation of suction pods 22, along the x-axis, by rotation of wheel 5. This spreading/closing action can be performed when the articulating arm 20 is either loose or tight. Additionally, when articulating arm 20 is loose, suction pods 22 can be independently rotated about the yz plane. This allows the surgeon wide flexibility in the manner of approach to the anastomosis site. Because the spreading action is parallel, the cardiac tissue tensioning effect is uniform across the anastomosis site (below and between suction pods 22).

Cable 40 terminates at tabbed element 4 by cable ball 50. Tensioning of cable 40 causes tabbed element 4 to move proximally. Ears 51 of tab element 4 mate into slot 52 of sling 10. Thus, tensioning or pulling on cable imparts tension or pulling back on sling 10. Sling 10 wraps around two pod guides 6, capturing guides 6 against head link 3. As cable 40 is tightened, sling 10 pulls pod guides 6 ever more firmly into head link 3 until they can no longer rotate. In the preferred embodiment, pod guides 6 are configured with square holes. These square holes are provided to mate with square projections on the pod guides and thus guide the movement of suction pods 22 in and out. The square shape serves to

prevent rotation of suction pods 22 in the yz plane once cable 40 has been tightened. Additionally, to prevent minor oscillations of suction pods 22 in the yz plane due to small clearances between pod guides 6 and suction pods 22, pod guides 6 each include small torsion springs 10 which bias suction pods 22 to one side of the respective pod guide 6. Suction pods 22 have a square element, which projects into the center of the spreader mechanism through pod guides 6.

Wheel 5 is located between the two pod guides 6. Wheel 5 has a threaded rod projecting through its center along the x-axis. To one side of wheel 5, the threaded rod has a right hand thread, and to the other side, a left hand thread. These threads mate with respectively threaded holes in the projections of the two suction pods 22. Rotating wheel 5 causes the pods to move simultaneously apart or together in parallel. Vacuum connections to suction pods 22 are made via barbed connections 25 at the proximal end of suction pods 22.

FIG. 6 is a perspective view of the second of three preferred embodiments for tightening/spreading mechanism 21. **FIG. 7** is an exploded perspective view of the tightening components of **FIG. 6**. The embodiment of **FIGS. 6 and 7** provides sequential tightening of the articulating arm concurrently or closely followed by angular separation of suction pods 22 in the xy plane, by tightening of handle 23. When articulating arm 20 is loose, suction pods 22 are free to rotate in the yz plane, and to a lesser extent in the xz and xy planes. This allows the surgeon even greater flexibility on approaching the anastomosis site. The tightening of cable 40 causes the spreading action. Because the spreading action is rotational, the tensioning effect will be uneven, being generally V-shaped, that is more pronounced at the distal end of the anastomosis site.

Cable 40 terminates in tabbed element 13. Tensioning of the cable causes the tabbed element to move proximally, pulling back on sling 14. The sling wraps around the split ball 225 of pods, capturing the split ball. In its relaxed state, when the stainless cable is loose, relatively little friction exist between

split ball 225, inner cavity of sling 14 and outer spherical surface of head link 12 so that split ball 225 is relatively able to be moved or rotated therein. In the preferred embodiment, the outside diameter of split ball is equal to the diameter of the spherical cavity defined within sling and head link, preferably these diameters are all approximately 0.193 inches. As the cable is tightened, however, the sling cinches down over the split ball compressing the split ball into the sling and head link 12. As the split ball 225 is compressed, the split 226 closes, causing suction pods 22 to splay angularly outward. In the preferred embodiment split ball 225 is made from non-glassed filled Ultem™ (available from GE Plastics, Pittsfield, Massachusetts.)

In a preferred embodiment, a compressible (preferably elastomeric) disk 15, is mounted between sling 14 and head link 12. The preferred material for disk 15 is silicone with a durometer of 80, although other materials or durometers or both may also be selected. Disk 15 preferably sits or mates into a compression limiter 41, depicted here as a stainless steel cup 41, which functions to limit the total amount to which the disk may be compressed. That is, disk 15 is sized to fit within cup so as to be able to be compressed an amount no greater than the depth of the cup. In the preferred embodiment, allowed to be compressed approximately no more than 0.040 inches. Of course, other sizes and material may also be selected. The identity, size, and other materials properties of the elastomeric disk 15 and cup (if used, for example, cup could be integrated into head link or cable tab) are chosen such that disk 15 it is crushed between head link 12 and sling 14 before the split ball is compressed. This causes articulating arm 20 to become firm before the spreading or other moving of the suction pods 22 begins, adding a desired degree of control to the system. Vacuum connections to suction pods 22 are made via barbed connections 25 at the proximal end of suction pods 22.

FIG. 8 is a perspective view of the third of three preferred embodiments for tightening/spreading mechanism 21. **FIG. 9** is an exploded perspective view of the tightening

components of **FIG. 8**. The embodiment of **FIGS. 8 and 9** provides independent rotational spreading of the suction pods (not shown in these two **FIGS.**) in any plane about a point of rotation at the center of the mechanism. When articulating arm 20 is loose, the suction pods 22 will move freely. Because the suction pods 22 are not linked together in this embodiment, they are able to conform to surfaces of the heart where the suction pods would not be co-planar. This provides more secure mounting of the suction pods on areas of the heart with small radii of surface curvature.

Cable 40 terminates at tabbed element 17. Tensioning of the cable causes tabbed element 17 to move proximally, pulling back on sling 18 through the interaction of ears 51 and groove 52. Pod mounts 19 EACH contain hemispherical sockets that fit smoothly about ball 50 and are captured between sling 18 and head link 16. Tensioning of cable 40 causes tabbed element 17 to move proximally, pulling back on sling 18, pinching ball 50 and the pod elements firmly together. In use, the surgeon would partially tighten the cable, and then pinch together the pod finger tabs 27 to achieve the desired amount of spreading. In a preferred embodiment, a compressible disk is used as described previously. Vacuum connections to the suction pods are made via barbed connections 25.

FIG. 10 depicts the relationship between rigidity of the articulating arm and the spreading apart of the suction pods 22 shown above in **FIG. 1-1**. As seen the present invention is designed so to provide a particular relationship between the rigidity of articulating arm and the spreading of suction pods. In the embodiment shown in **FIGS 6 & 7** the initial relationship between rigidity and spread is linear until a spreading point, seen here as Q, is reached. Thereafter a non-linear relationship is seen. In this embodiment there is thus a simultaneous change in the rigidity of the arm and the spreading of the pods.

FIGS. 11 & 12 depict the relationship of rigidity and spreadability in a further embodiment of the present invention. As seen in this embodiment the articulating arm undergoes a transformation of

rigidity from loose flexibility to firm flexibility at time B_1 . Thereafter, at time B_2 articulating arm undergoes a transformation of rigidity from firm to hard. Continuing tightening of the handle (which controls rigidity and spread in the embodiment shown in FIGS. 1-7) does not cause the arm to become appreciatively more rigid. In contrast, the spreadability of the suction pods is depicted in FIG. 12 and is seen, in particular, to occur at a lag from the transformation of rigidity. In particular, as seen at B_1 the rigidity is increased from loose to firm while the spread of the suction pods does not occur until time C_1 that is, turning of handle 23 to reduce the flexibility of the part of the articulating arm from loose to firm does not cause an appreciable spread until a time thereafter, here seen as C_1 . The particular relation between rigidity and spread may be selected to occur in any favorable matter. Practically speaking, the relationship between rigidity and spread may be a matter of choice which is best left to the surgeon. Thus, the present invention permits this relationship to be tailored as desired though the selection of among the following factors: in the present invention shown in FIG. 1-1 and thereafter shown in particular regard in FIGS. 6 & 7, the relationship of rigidity and spread may be controlled through the particular design and selection of the arm links and texture, split ball and hinge, split ball and split or gap, washer and cup as well as any of their materials.

This is seen in FIGS. 13 through 21, which show the split ball 225 of the preferred embodiment (FIG. 13 through 16) and alternative designs. As seen FIG. 13 is a detailed perspective of split ball 225 shown assembled in a stabilization system. FIG. 14 is a plan view of the split ball 225 shown in FIG. 13 from an overhead position. This view shows the split or gap 226 within split ball and the hinge 227. The size of hinge 227 and split or gap 226 define the actuation of the pods mounted to the split ball and further the degree of force required. These elements, along with other elements of the present invention, may be tailored to provide the particular actuation and performance characteristics deemed suitable for a surgeon or surgeons. FIG. 15 is a cross sectional view of split ball 225 shown in

FIG. 13 along line 15-15. In the preferred embodiment gap 226 has a minimum thickness T_{226} of between 0.010 – 0.100 inches, with 0.040 inches preferred, while hinge 227 has a thickness T_{227} of between 0.220 – 0.010 inches, with 0.110 inches preferred. **FIG. 16** is a two-dimensional plot of the gap along the outer surface of the split ball. As seen, in this embodiment, gap is symmetrical along the outer surface.

Many other alternative embodiments of the split ball may be provided. **FIG. 17** shows one embodiment in which the hinge is positioned above the center line of the split ball. **FIG. 18** shows one embodiment in which the hinge is positioned below the center line of the split ball. **FIG. 19** shows one embodiment in which the hinge is positioned at the backside of the split ball, as compared to the embodiment seen in **FIG. 15**. In this embodiment the tension on the cable would cause the front of the split ball to be compressed, thereby spying inwardly the suction pods. Such pod movement may be useful for squeezing tissue between the pods. Besides positioning the gap and thus the hinge at various portions within the split ball, gap may further be fashioned so as to be larger at a top end and smaller or narrower at a bottom end. **FIG. 20** shows an embodiment in which gap 227 is wider at the upper end (above the 0 degree line) and narrower at the lower end (below the 0 degree line). **FIG. 21** is a two-dimensional plot of the gap along the outer surface of the split ball. As seen, in this embodiment, gap is non-symmetrical along the outer surface, larger at its upper end and narrower in its bottom end.

FIG. 22 depicts an alternative embodiment of the present invention. In this embodiment suction pods are separated, and not joined such that each suction pod is free to be moved within the Y Z plane, similar to that already shown in **FIG. 4**. Movement is provided through the segmented spreadable hinge 199, which is provided through the interrelationship of sling 15 and the corresponding left suction pod 22L and right suction pod 22R. Spreadable hinge 199 is provided through an inter-mating ball and socket assembly, provided on respective floating pods 22R and 22L in particular a

hemispherical ball 198 is provided on right suction pod 22R and a corresponding inter-mating hemispherical socket 197. As seen socket and ball are dimensioned such that they may be mated together and the smaller diameter portion of ball inserted into the hemispherical opening of hemispherical socket 197. Thereafter the mated together pieces generally form a segmented hemisphere which may be disposed within the sling 15 as already described above in regards to **FIGS. 6 & 7**. This embodiment has advantages over that shown above in **FIGS. 6 & 7** because the individual paddles 22L & 22R may be oriented along the various axis to provide secure capture of the surface of the heart.

In a further embodiment of the present invention the segmented spreadable hinge 199 as well as spreadable hinge shown above in regards to **FIGS. 6 & 7** may be provided such that the suction pods move in a non-parallel fashion. One embodiment of this non-parallel movement is shown in **FIG. 23**. As seen in a first, non-spread, orientation paddle 22L & 22R are disposed of first distance A apart. Once the spreading has been ignited through any of the various methods described above, paddles 22L & 22R shown on the disposition of **FIG. 24**. As seen in this disposition the closes point the paddles have to one another is at their base or proximal positions and is at a distance $A + X$. The distal ends of the paddles are shown at a distance $A + Y$ apart such that an angle faded exists between the longitude and the axis of each paddle. Embodiments which may be utilized to achieve this movement are those shown above.

FIG. 30 depicts further alternative embodiment of the present invention. In this embodiment suction pods 22L & 22R may be spread and rotated such that they move from an orientation shown in **FIG. 30**, and have a distance A apart, to the orientation shown in **FIG. 31**. As seen in **FIG. 31**, at this point paddles 22L & 22R are a minimal distance $A + X_1$ apart at their proximal end an greater distance

A+X2 apart at their distal end. Furthermore, the pods have had a relative rotation such that the bottom surface of the pods now define an angle σ .

FIG. 32 depicts a further alternative embodiment of the present invention. In particular, **FIG. 32** is a sectional view across pod 22L shown in **FIG. 22** along line O-O. As seen, in this embodiment, pod 22L features a suction port 33 open along the bottom surface of the suction pod. Suction port 33 further communicates with a suction aperture 31. In this embodiment the total height H of the pod is minimized because the suction aperture is located along side the suction port such that the aperture exists at the point at the suction port no greater than the alternate height of the suction port opening, that is the bottom of the suction port, depicted here as 33-b is relatively above, in this figure, suction aperture 34. This is between approximately 1 and 4 millimeters, with 2-3 preferred.

FIGS. 33-37 depict alternative embodiments of the suction pods. These alternative embodiments may be used together or in any combination of any of the above and below shown suction pods. Exact usage of these types of suction pods would be at the preference of the surgeon. In **FIG. 33** an embodiment is shown in which each of the suction ports 33-1 through 33-5 have the same diameter. In this embodiment, however, the suction apertures 34-1 through 34-4 have different opening sizes into the relative suction ports. In particular, in this embodiment suction aperture 34-2 and 34-3 are relatively much larger than the corresponding suction apertures 34-1 and 34-5. The relatively larger suction apertures are provided in that they provide a more quick capture and fixation of the relevant suction port to the tissue. In contrast, suction ports having relatively smaller suction apertures require more time to effectively capture the tissue. While shown in this **FIG. 33** as having relatively larger suction apertures in the two central ports, the opposite may also be provided such that the relatively larger suction apertures are at the end suction ports. The benefit of this configuration is

that ports 33-1 and 33-4 are least likely to spontaneously lose capture, while the inner ports 33-2 and 33-3 will quickly achieve capture.

FIG. 34 shows an additional embodiment of the present invention. In this embodiment suction pod is non-rectangular, and in particular, shown as having a relatively, tapered, elongated orientation. Furthermore, such ports are provided which have variable diameters. In particular, in this embodiment, suction port 33-1 has relatively larger diameter, and the diameter of the subsequent suction ports 33-2 at Et seq. become relatively smaller until suction port 33-5 as shown as having the smallest suction port diameter. In this embodiment the corresponding suction apertures 34-1 through 34-5 are provided having a consistent diameter and those surface area opening into the suction ports. Of course, as described above these may be varied in size.

FIG. 35 shows a suction pod having an ever decreasing sized suction ports and furthermore having ever decreasing sized apertures and ports.

While suction port has been shown above as generally circular it may also be provided in other, non circular forms. In **FIG. 36** it is shown that suction port may be provide both as elliptical as well as trapezoidal configurations. In each of the embodiments suction port is provided with a single suction aperture. Of course, suction aperture may be provided more than once into the same suction port.

FIG. 37 shows a suction pod having variable diameter suction ports while consistent suction apertures. In this embodiment the central suction port are much larger than the end point suction ports.

FIGS. 38-40 depict an alternative embodiment of the present invention. As seen, suction pod 22 has a series of suction ports 33 as already described above. In this embodiment suction pod is made, however, from a malleable material such that the pod itself can be shaped by the surgeon prior to disposition of the pod onto the surface of the heart. It is believed that this malleability provides the surgeon with increased flexibility so as to shape the pod to be conformed into or around the surface of

the particular area of the heart upon which he will operate. As seen malleable pod may further include a spring or other form of malleable but lockable member 190. In the present invention this lockable member 190 would comprise a wound coiled spring, although other materials and devices may be used, including, but not limited to, straps, band, bands, interwoven metallic members, heat set plastics, to name some of other alternative materials and devices which may be used. In a first embodiment the malleable pod is constructed of PVC (poly vinyl chloride) 73 Shore A durometer and the lockable member is constructed from a hypotube made of MP35N metal alloy. In the preferred embodiment the hypotube used to carry suction to the suction ports and thus functions as a suction aperture. Alternately, the malleable pod formation permits the pod itself to be moved from its first orientation, as seen in **FIG. 40** at 189 to the deformed position 188 shown at **FIG. 40**. Alternatively, pod may be manufactured from many other types of materials, including silicone rubber, polyurethane, to name only a few, while lockable member may be constructed from coiled conductors, polymeric strips, or strips or ribbons or springs made from nitinol.

The present invention may be especially suitable for performing a surgical operation on a patient utilizing the simultaneous spreading of the device' paddles and the stiffening of the fixation arm. That is, this embodiment may permit use of the following method of performing a surgical procedure. First, the desired area of tissue is accessed, e.g. the heart and the coronary artery of interest is accessed. Next, a stabilization system is placed upon the surface of the tissue, e.g. a stabilization system as shown in **FIGS. 1-3, 6-9** is placed upon the surface of the tissue, and in particular suction pods 22 is placed upon the surface of the tissue. Next, suction is introduced into each pod such that the surface of the tissue is captured by the first pod and the second pod. Next, the first pod and the second pod are caused to be spread relatively apart while the articulating arm 20 is concurrently caused to become stiff. In the illustrated embodiment of **FIGS. 1-3** this may be accomplished by turning distal

handle 23. As already described above, turning of distal handle causes tension to be applied to cable, causing in turn first paddle and second paddle to thereafter be spread relatively apart or otherwise moved (e.g. moved together, where the exact motion depends on the hinge design and the orientation of the pods or paddles) and also causing each of the links of the arm to be compressed together. The method may also be performed where the step of causing the articulating arm to become stiffer may be performed at either a time prior to or after the step of spreading relatively apart the first pod and the second pod. Thereafter a surgical procedure may be performed. Finally, the process is reversed and the patient is closed, as is well known in the art.

The particular embodiment shown in **FIGS. 4 and 5** may be especially suitable for performing a surgical operation on a patient utilizing only the spreading aspect of the device' paddles and not the stabilization through the stiffening of the fixation arm. That is, this embodiment may permit use of the following method of performing a surgical procedure. First, the desired area of tissue is accessed, e.g. the heart and the coronary artery of interest is accessed. Next, a stabilization system is placed upon the surface of the tissue, e.g. a stabilization system as shown in **FIGS. 4 and 5** is placed upon the surface of the tissue, and in particular suction pods 22 is placed upon the surface of the tissue. Next, suction is introduced into each pod such that the surface of the tissue is captured by the first pod and the second pod. Next, the first pod and the second pod are caused to be spread relatively apart. In the illustrated embodiment this may be accomplished by turning wheel 5 to cause first paddle and second paddle to thereafter be spread relatively apart. Thereafter a surgical procedure may be performed. Finally, the process is reversed and the patient is closed, as is well known in the art. Thus this method does not require the use of a stiffened arm to provide for the further stabilization. Only the spreading of the paddles is used.

In a further embodiment, the system may be further configured to feature paddles which do not feature suction ports for capturing tissue. Rather, in this embodiment, shown in **FIG. 41** frictional engagement only by the bottom surface of the paddles is used along with the spreading action to stabilize the tissue. All other aspects of this embodiment may be the same as shown already above. In a further alternative of this design, the tissue-contacting bottom surfaces of the paddles may be treated with materials or textures or both to enhance the friction or gripability between the tissue and the paddle. These embodiments may thus be used to perform a method of performing a surgical procedure upon a patient along the following steps of. First, a desired area of tissue on a patient is accessed. Next, a stabilization system having an articulating arm, the articulating arm having a first pod and a second pod is provided. Preferably one or more of the pods has a bottom surface shaped to conform to the surface of the heart, and further the tissue-contacting bottom surfaces of the paddles are treated with materials or textures or both to enhance the friction. Next the stabilization system is placed upon the surface of the tissue. Next the first pod and the second pod are spread relatively apart. Next the desired surgical procedure is performed. Thereafter the system is removed and the patient is closed.

In a still further embodiment, shown here in **FIG. 42**, the bottom surface may feature a series of burrs or upraised barbs 656. These structures act as cleats which puncture or are introduced a small amount, between 0.25 to 1.5 millimeter beyond the surface of the tissue and into the tissue itself, more or less, and serve to enhance the friction or gripability between the tissue and the paddle. Moreover, still further, these structures may be made hollow and may be coupled to a dispensing reservoir containing drugs, agents or other desired medicinal substance (such as anti-clotting agents, clotting agents, steroids, anti-biotics, growth factors, genetically acting agents or anti arrhythmic agents, to name only a few) so as to also be used to inject directly such substances into the tissue in the vicinity

adjacent the surgical procedure. e.g. into the epicardium in the vicinity adjacent the anastomosis. Other than these features, all other aspects of this embodiment may be the same as shown already above.

FIG. 43 is a perspective view of an alternative embodiment for tightening/spreading mechanism 21. In this embodiment a series of spreadable wedges having a series of inclines which cooperate with a cable stop to provide a system wherein movement of the pos or paddles may be caused to occur concurrent with or following arm tightening. As seen cable stop 300 is positioned at the distal end of arm. Cable stop hold the distal end of cable, not seen in this **FIG.** Cable stop is generally a cube like structure, having a relatively sharp corner or edge which is disposed to ride along first inclined surface 303 or second inclined surface 305 of spreadable saddle 307. As seen first inclined surface 303 is disposed at a first angle on spreadable saddle while second inclined surface 305 is disposed at a second angle on spreadable saddle such that the first angle is relatively more flat or oblique in regards to the bottom surface of cable stop 300 when compared to the second angle. Through these inclines and their angular relation to the bottom surface and side edges of cable stop, the co-efficient of friction between the cable stop and the first inclined surface 303 and second inclined surface 305 will be different. In such a manner, a first tension to the cable will generally first cause the arm and its links to be pulled together, thereafter, once tension exceeds the required coefficient of friction and cable stop is moved to engage the second inclined surface will the spreadable saddle be caused to fully begin to spread. As can be seen, a hemispherical mounting 309 is disposed between saddle 307 and U-link 311 such that spreading of saddle pinches mounting and therefore causes movement of the attached pods or paddles (only one of which is depicted here in outline as 22.)

FIG. 44 is a perspective view of an alternative embodiment for tightening/spreading mechanism 21. In this embodiment spread or other movement of the pods or paddles may be accomplished through hydraulic actuation. While shown here as hydraulic actuation, it should also be

understood, as used herein, hydraulic also encompasses pneumatic actuation as well. As seen mechanism 21 features a spherical center hinge 400, which is used to couple the shown assembly to an articulated arm, as already described above. That is spherical center hinge 400 may be used in place of split ball. Left pod assembly 402 features a conventional connection 25 to permit suction to attached and communicated to a series of ports, as already described above. This embodiment further features a hydraulic actuator composed of the shaft 404 and seals 406, where the shaft is dimensioned to be slideably moved within runway 408 of left pod assembly. Stop 410 prevents excessive movement of shaft. While shaft itself is depicted as straight, it should be understood it could also be curved so that the right pod or paddle may be made to move in an arc. Runway 408 is coupled by a coupling 411 to hydraulic line 412, which in turn, is coupled to control valve 414 and hydraulic/pneumatic source 416.

FIG. 45 is a still further embodiment of the present invention. In this embodiment all other features are the same as those described above in regards to **FIG. 1** but for that the arm 420 is rigid, as opposed to the flexible arm shown above in **FIG. 1**. Rigid arm 420 may be used where the are in which the procedure is performed is extremely cramped. Arm 420, because it does not flex may have a much decreased diameter as compared to arm 20 (recall that the **FIGS.** Are not necessarily to scale.)

The present invention provides the following advantages over conventional suction stabilization systems. First, it reduces the force required to tighten and loosen the articulating arm(s). Second, it improves access to the surgical site in general due to its reduced size, and to the anastomosis site in particular due to the flexibility of the system components and geometry of the system components. Third, it permits relatively delicate manipulations to smoothly spread the suction pods without causing the suction pods to become detached form the arm. Fourth, use of a single arm to support multiple suction pods eliminates interference between opposing arms, such as occurred in the conventional systems when the surgeon tried to position the tissue stabilizers. Fifth, the time to set up

the equipment is significantly reduced. Sixth, the design reduces inconsistent performance due to improper maintenance, wear, or unreliable mounting surfaces.

As disclosed, the present invention relates to a method and apparatus for immobilizing tissue. In the preferred embodiment, the invention is used to immobilize heart tissue for a coronary artery bypass graft procedure using either an open or closed chest approach, without the need for a cardiopulmonary bypass. Other surgical techniques, however, which require immobilizing body tissue may also be performed using the present invention, such as surgery on other organs such as the stomach, gall bladder, etc., as well as on other body tissues, such as the eye or the skin, for example. In addition, while the present invention has been described in detail with particular reference to a preferred embodiment and alternative embodiments, it should be understood variations and modifications can be effected within the scope of the following claims. Such modifications may include substituting elements or components which perform substantially the same function in substantially the same way to achieve substantially the same result for those described herein.

WHAT IS CLAIMED IS

1. A system for temporarily immobilizing an area of tissue comprising a paddle assembly, paddle assembly having a first paddle and a second paddle, the paddle assembly further having means for spreading the first paddle away from the second paddle; an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm having means for permitting the arm to flex, the arm having means for fixing the arm to an object; and arm locking means coupled to the arm, the arm locking means permitting the locking of the arm in any selected position wherein the distal end of the arm is maintained in the selected position.
2. The system according to claim 1 wherein the first paddle has means for engaging heart tissue.
3. The system according to claim 2 wherein the means for engaging heart tissue further comprises at least a first suction port positioned along a first surface of the first paddle.
4. The system according to claim 3 wherein the means for engaging heart tissue further comprises at least a second suction port positioned along a second surface of the second paddle.
5. The system according to claim 4 wherein the first surface and the second surface are generally within the same plane.
6. The system according to claim 5 further comprising the first paddle is adapted to have a first surface which conforms to the surface of the heart.
7. The system according to claim 2 wherein the means for engaging heart tissue further comprising a series of ridges along the first paddle lower surface.

8. The system according to claim 1 further comprising the first paddle is adapted to have a first surface which is conformable to the surface of the heart.
9. The system according to claim 8 wherein the first paddle is constructed of a malleable material.
10. The system according to claim 9 wherein the first paddle further comprises a stiffening element therein.
11. The system according to claim 10 further comprising at least a first suction port positioned along a first surface of the first paddle.
12. The system according to claim 1_ wherein the first paddle has at least one first suction port and the second paddle has at least one second suction port.
13. The system according to claim 12_ further comprising a suction source.
14. The system according to claim 13_ wherein the first paddle has means for coupling the at least one first suction port to the suction source.
15. The system according to claim 14_ wherein the means for coupling are positioned along a proximal end of the first paddle
16. The system according to claim 12_ wherein the means for coupling further comprising a first nozzle adapted to be inserted into a polymeric tube.
17. The system according to claim 12_ wherein the means for spreading comprises:
a cable stop coupled to distal end of arm, the arm having a cable running therethrough, a distal end of cable coupled to cable stop

a spreadable saddle coupled to distal end of arm, the spreadable saddle having a first inclined surface, wherein the cable stop will slide upon the first inclined surface as the cable receives a first amount of tension and the spreadable saddle is spread a first amount.

18. The system according to claim 17_ wherein the spreadable saddle further comprises a second inclined surface, wherein the cable stop will slide upon the second inclined surface as the cable receives a second amount of tension and the spreadable saddle is spread a second amount.

19. The system according to claim 17_ further comprising a link disposed upon the distal end of the arm such the link is mounted between the arm and the saddle, a paddles mounting disposed between the link and the saddle.

20. The system according to claim 12_ wherein the cable stop further comprises a generally cube like structure.

21. The system according to claim 20_ wherein the means for spreading the first paddle and second paddle apart further comprises a hydraulic cylinder disposed upon the distal end of the arm, the first pod mounted to a first end of a first shaft couple to the hydraulic cylinder and the second pod mounted to a second shaft coupled to the second end of the cylinder.

22. The system according to claim 21_ further comprising a hydraulic reservoir and valve, the reservoir and valve providing hydraulic actuation of the hydraulic cylinder wherein the first paddle may

be made to move relative to the second paddle through movement of hydraulic fluid from the hydraulic reservoir to the hydraulic cylinder.

23. The system according to claim 22_ wherein the second shaft is curved wherein movement of the second paddle relative to the first paddle occurs in an arc.

24. The system according to claim 1_ wherein the means for spreading further comprise means for independently spreading the first paddle and second paddle apart.

25. The system according to claim 24_ wherein the means for independently spreading the first paddle and second paddle apart in a generally parallel relation are positioned upon the distal end of the arm.

26. The system according to claim 25_ wherein the means for independently spreading the first paddle and second paddle apart further comprising a spreader (wheel), the spreader having a first screw, the first screw engaging with a first threaded hole in the first pod wherein movement of the spreader causes the first paddle to be moved in an axial direction along the first screw.

27. The system according to claim 26_ further comprising the spreader having a second screw, the second screw engaging with a second threaded hole in the second pod wherein movement of the spreader causes the second paddle to be moved in an axial direction along the second screw.

28. The system according to claim 26_ further comprising the spreader having a second screw, the second screw engaging with a second threaded hole in the second pod wherein movement of the spreader causes the second paddle to be moved in direction parallel to the first paddle.
29. The system according to claim 24_ further comprising a first means for biasing the first paddle away from the spreader, the means for biasing disposed adjacent the first paddle.
30. The system according to claim 29_ wherein the first means for biasing the first paddle away from the spreader further comprises a torsion spring disposed about the first screw so as to bias the first paddle away from the spreader.
31. The system according to claim 29_ further comprising a second means for biasing the first paddle away from the spreader, the means for biasing disposed adjacent the first paddle.
32. The system according to claim 31_ wherein the second means for biasing the first paddle away from the spreader.
33. The system according to claim 31_ further comprising a torsion spring disposed about the second screw so as to bias the first paddle away from the spreader.
34. The system according to claim 1_ wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle a parallel relation.

35. The system according to claim 1 _ wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle in a non parallel relation.

36. The system according to claim 1 _ wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge

37. The system according to claim 36_ wherein the spreadable hinge is coupled to the arm locking means.

38. The system according to claim 37_ wherein the spreadable hinge is coupled to the arm locking means by a cable wire.

39. The system according to claim 38_ wherein the cable is stranded.

40. The system according to claim 37_ wherein the spreadable hinge further comprising a split ball, a first end of the split ball coupled to the first paddle, a second end of the split ball coupled to the split ball.
41. The system according to claim 40_ wherein the split ball is adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the split ball is dimension to be pressured by the sling in the second position, the split ball further sized to be spread apart due to the force exerted upon it by the sling.
42. The system according to claim _ further comprising a head link positioned at the distal end of the arm wherein the split ball is adapted to be mated into the retention sling and against the head link.
43. The system according to claim 40_ wherein the split ball has a split, the split symmetrical about a first plane.
44. The system according to claim 43_ wherein the split ball has a split, the split symmetrical about a second plane.
45. The system according to claim 44 _ wherein the split ball has a split, the split symmetrical about a first plane which is non-parallel to a major plane of the paddle assembly.
- 46. The system according to claim _ wherein 1 the means for spreading the first paddle and second paddle apart further comprising a segmented spreadable hinge.**
47. The system according to claim 46_ wherein the segmented spreadable hinge is coupled to the arm locking means.

48. The system according to claim 47_ wherein the segmented spreadable hinge further comprises a intermating ball and socket assembly,

49. The system according to claim 48_ wherein the intermating ball and socket assembly further comprises a first ball having a first end and a hemisphere having a second end, the first end of the first ball coupled to the first paddle, the second end of the hemisphere coupled to the second paddle.

50. The system according to claim 49_ wherein the hemisphere has a hollow, the first end of the first ball is sized to be mated into the hollow.

51. The system according to claim 50_ wherein the first ball mated into the hemisphere are further adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the first ball and the hemisphere are dimension to be pressured by the sling in the second position wherein the first ball rotates relative to the hemisphere

52. The system according to claim 51_ further comprising a head link positioned at the distal end of the arm wherein the first ball and the hemisphere are adapted to be positioned into the retention sling and against the head link.

53. The system according to claim 1_ wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart

54. The system according to claim 53_ further comprising means for simultaneously rotating the first paddle along its first major axis in a first direction.

55. The system according to claim 54_ further comprising means for simultaneously rotating the second paddle along its second major axis in a second direction.

56. The system according to claim 55_ wherein the first direction is opposite the second direction.
57. The system according to claim 1_ wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position, wherein in the first position the first paddle and second paddle are configured in a parallel relation.
58. The system according to claim 57_ wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position, _ wherein in the second position the first paddle and second paddle are configured in a parallel relation.
59. The system according to claim 1_ wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position,
60. The system according to claim 59_ wherein in the first position the first paddle and second paddle are configured in a non parallel relation.
61. The system according to claim 60_ wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position,
62. The system according to claim 60_ wherein in the second position the first paddle and second paddle are configured in a non parallel relation.
63. The system according to claim 1_ wherein the first paddle has a first surface, a first suction port positioned within the first surface, a second suction port positioned within the first surface, a third suction port positioned within the first surface

64. The system according to claim 63_ wherein the first suction port, the second suction port, and the third suction port are all in a linear relation.

65. The system according to claim 64_ further comprising a suction source, the first suction port coupled to the suction source through a first suction aperture, the first suction aperture having a first suction aperture surface area.

66. The system according to claim 65_ further comprising a suction source, the second suction port coupled to the suction source through a second suction aperture, the second suction aperture having a second suction aperture surface area.

67. The system according to claim 66_ further comprising a suction source, the third suction port coupled to the suction source through a third suction aperture, the third suction aperture having a third suction aperture surface area.

68. The system according to claim 66_ wherein the first suction aperture surface area is different from the second suction aperture surface area.

69. The system according to claim 68 wherein the third suction aperture surface area is different from the second suction aperture surface area.

70. The system according to claim 64_ wherein the first suction port has a non- circular shape within the first plane.

71. The system according to claim 64_ wherein the non-circular shape within the first plane is an ellipse.

72. The system according to claim 64_ wherein the non-circular shape within the first plane is a trapezoid.

73. The system according to claim 64_ wherein the non-circular shape within the first plane is a square.

74. The system according to claim 64_ wherein the first suction port is larger than the second suction port

75. The system according to claim 74_ wherein the first suction port is disposed closer to the proximal end of the first paddle than the second suction port.

76. The system according to claim 75_ wherein the second suction port is larger than the third suction port.

77. The system according to claim 75_ wherein the second suction port is smaller than the third suction port.

78. The system according to claim 1_ wherein the first paddle has a rectangular cross section along a first plane.

79. The system according to claim 1_ wherein the first paddle has a triangular cross section along a first plane.

80. The system according to claim 1_ further comprising the first paddle has a first surface, a first suction port positioned within the first surface, a suction source, the first suction port coupled to the suction source through a first suction aperture, the first suction port having a bottom opening within the first surface and an upper surface within the first paddle, the suction aperture positioned within the first paddle between the first surface of the first paddle and the upper surface of the first suction port.

81. The system according to claim 1_ wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart
82. The system according to claim 1_ wherein the arm has a series of articulations wherein the arm may be bent along a curved arc among a plurality of direction.
83. The system according to claim 82_ wherein the series of articulations are provided through a series of interlocking links.
84. The system according to claim 83_ wherein at least one first link in the series of interlocking links has a first hemispherical surface having a first hemispherical diameter and at least one second link in the series of interlocking links has a second hemispherical indentation having a second hemispherical diameter.
85. The system according to claim 84_ wherein the first diameter is equal to the second diameter.
86. The system according to claim 85_ wherein the at least one first link has a first center lumen therethrough and the at least one second link has a second center lumen therethrough, the first link and the second link coupled through a first tensioning element disposed within the respective center lumens.
87. The system according to claim 1_ wherein the means for spreading the first paddle away from the second paddle further comprises a tensioning element running from a proximal end of the arm to the distal end of the arm.

88. The system according to claim 87_ wherein the cable running from a proximal end of the arm to the distal end of the arm is a stranded cable.
89. The system according to claim 1_ wherein the arm comprises a series of interlocking links, each link having a hemispherical protrusion and a hemispherical indentation,
90. The system according to claim 89_ wherein the links are constructed from a polymer.
91. The system according to claim 90_ wherein the polymer comprises a glass fiber filled thermoplastic.
92. The system according to claim 91_ wherein a surface of the hemispherical protrusion and a surface of the hemispherical indentation has a roughened texture.
93. The system according to claim 89_ wherein a surface of the hemispherical protrusion and a surface of the hemispherical indentation has a series of interlocking dimples and depressions.
94. The system according to claim 1'_ wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed on the proximal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.
95. The system according to claim 94_ wherein the spreading actuator further comprises a torque screw.

96. The system according to claim 1_ wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed away from the distal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.

97. The system according to claim 96_ wherein the spreading actuator further comprises a torque screw.

98. The system according to claim 96_ wherein the spreading actuator further comprises a hydraulic reservoir.

99. The system according to claim 89_ wherein the first hemispherical surface has a series of first protrusions of a first protrusion shape.

100. The system according to claim 99_ wherein the second hemispherical indentation has a series of second indentations of a second indentation shape.

101. The system according to claim 100_ wherein the first protrusions are substantially the same size as the second indentations.

102. The system according to claim 100_ wherein the first hemispherical surface has a series of first indentations of a first indentations shape.

103. The system according to claim 100_ wherein the second hemispherical indentation has a series of second protrusions of a second protrusions shape.

104. The system according to claim 1 wherein the first paddle having a first bottom surface shaped to engage the surface of the tissue,

- 105 The system according to claim 104_ wherein the first bottom surface further comprises a series of tissue puncturing cleats.
- 106 The system according to claim 105_ wherein the series of tissue puncturing cleats extend for a distance between 0.25 and 1.0 millimeter from the first bottom surface.
- 107 The system according to claim 105_ wherein the series of tissue puncturing cleats are hollow
- 108 The system according to claim 107_ wherein the series of tissue puncturing cleats are coupled to a dispensing reservoir.
- 109 The system according to claim 108_ wherein the dispensing reservoir contains a medicinal substance.

This is an alternative claim NOT HAVING ARM LOCKING but still having arm spreading.

WE NEED TO DESCRIBE THE SYSTEM AND METHOD OF USING THIS DEVICE

110. A system for stabilizing tissue comprising

a paddle assembly, paddle assembly having a first paddle and a second paddle. the paddle assembly further having means for spreading the first paddle away from the second paddle;

an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm having means for permitting the arm to flex, the arm having means for fixing the arm to an object;

111. The system according to claim 110 further comprising arm locking means coupled to the arm. the arm locking means permitting the locking of the arm in any selected position wherein the distal end of the arm is maintained in the selected position.

112. The system according to claim 111 wherein the first paddle has means for engaging heart tissue.

113. The system according to claim 112 wherein the means for engaging heart tissue further comprises at least a first suction port positioned along a first surface of the first paddle.

114. The system according to claim 113 wherein the means for engaging heart tissue further comprises at least a second suction port positioned along a second surface of the second paddle.

115. The system according to claim 114 wherein the first surface and the second surface are generally within the same plane.

116. The system according to claim 115 further comprising the first paddle is adapted to have a first surface which conforms to the surface of the heart.

117. The system according to claim 110 wherein the first paddle has at least one first suction port and the second paddle has at least one second suction port.

118. The system according to claim 110_ further comprising a suction source.

119. The system according to claim 118_ wherein the first paddle has means for coupling the at least one first suction port to the suction source.

120. The system according to claim 119_ wherein the means for coupling are positioned along a proximal end of the first paddle.

121. The system according to claim 110 wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle a parallel relation.

122. The system according to claim 110 wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle in a non parallel relation.

123. The system according to claim 110_ wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge

124. The system according to claim 123_ wherein the spreadable hinge is coupled to the arm locking means.

125. The system according to claim 124_ wherein the spreadable hinge is coupled to the arm locking means by a cable wire.

126. The system according to claim 125_ wherein the cable is stranded.

136. The system according to claim 124 wherein the spreadable hinge further comprising a split ball, a first end of the split ball coupled to the first paddle, a second end of the split ball coupled to the split ball.

137. The system according to claim 136_ wherein the split ball is adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the split ball is dimension to be pressured by the sling in the second position, the split ball further sized to be spread apart due to the force exerted upon it by the sling.

138. The system according to claim 137_ further comprising a head link positioned at the distal end of the arm wherein the split ball is adapted to be mated into the retention sling and against the head link.

139. The system according to claim 110_ wherein the split ball has a split, the split symmetrical about a first plane.

140. The system according to claim 139_ wherein the split ball has a split, the split symmetrical about a second plane.

141. The system according to claim 140_ wherein the split ball has a split, the split symmetrical about a first plane which is non-parallel to a major plane of the paddle assembly.

142. The system according to claim 110_ wherein 1 the means for spreading the first paddle and second paddle apart further comprising a segmented spreadable hinge.

143. The system according to claim 110_ wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart

144 The system according to claim 143 further comprising means for simultaneously rotating the first paddle along its first major axis in a first direction.

145. The system according to claim 144 further comprising means for simultaneously rotating the second paddle along its second major axis in a second direction.

146. The system according to claim 145_ wherein the first direction is opposite the second direction.

147. The system according to claim 110_ wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position, wherein in the first position the first paddle and second paddle are configured in a parallel relation.

148. The system according to claim 110_ wherein the first paddle has a first surface, a first suction port positioned within the first surface, a second suction port positioned within the first surface, a third suction port positioned within the first surface

149. The system according to claim 148_ wherein the first suction port, the second suction port, and the third suction port are all in a linear relation.

150. The system according to claim 110_ further comprising the first paddle has a first surface, a first suction port positioned within the first surface, a suction source, the first suction port coupled to the suction source through a first suction aperture, the first suction port having a bottom opening within the first surface and an upper surface within the first paddle, the suction aperture positioned within the first paddle between the first surface of the first paddle and the upper surface of the first suction port.

151. The system according to claim 111_ wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart

152. The system according to claim 110_ wherein the arm has a series of articulations wherein the arm may be bent along a curved arc among a plurality of direction.

153. The system according to claim 152_ wherein the series of articulations are provided through a series of interlocking links.

154. The system according to claim 110_ wherein the means for spreading the first paddle away from the second paddle further comprises a tensioning element running from a proximal end of the arm to the distal end of the arm.

Claims for the needle and injection paragraphs

155. A system for temporarily immobilizing an area of tissue comprising a paddle assembly, paddle assembly having a first paddle and a second paddle, the first paddle having a first bottom surface shaped to engage the surface of the tissue, the bottom surface having means to

enhance the friction between the tissue and the paddle bottom surface, the paddle assembly further having means for spreading the first paddle away from the second paddle;
an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm having means for permitting the arm to flex, the arm having means for fixing the arm to an object; and
arm locking means coupled to the arm, the arm locking means permitting the locking of the arm in any selected position wherein the distal end of the arm is maintained in the selected position.

156. The system according to claim 155 the first paddle having a first bottom surface shaped to engage the surface of the tissue,

157. The system according to claim 155 the first bottom surface further comprises a series of tissue puncturing cleats.

158. The system according to claim 155 wherein the first paddle has means for engaging heart tissue.

159. The system according to claim 158 wherein the means for engaging heart tissue further comprises at least a first suction port positioned along a first surface of the first paddle.

160. The system according to claim 159 wherein the means for engaging heart tissue further comprises at least a second suction port positioned along a second surface of the second paddle.

161. The system according to claim 160 wherein the first surface and the second surface are generally within the same plane.

162. The system according to claim 160 further comprising the first paddle is adapted to have a first surface which conforms to the surface of the heart.

163. The system according to claim 155 wherein the means for spreading further comprise means for independently spreading the first paddle and second paddle apart.

164. The system according to claim 155 _ wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge

165. The system according to claim 164_ wherein the spreadable hinge is coupled to the arm locking means.

166. The system according to claim 164_ wherein the spreadable hinge further comprising a split ball, a first end of the split ball coupled to the first paddle, a second end of the split ball coupled to the split ball.

167. The system according to claim 166_ wherein the split ball is adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the split ball is dimensioned to be pressured by the sling in the second position, the split ball further sized to be spread apart due to the force exerted upon it by the sling.

168. The system according to claim 167_ further comprising a head link positioned at the distal end of the arm wherein the split ball is adapted to be mated into the retention sling and against the head link.

169. The system according to claim 166_ wherein the split ball has a split, the split symmetrical about a first plane.

170. The system according to claim 169_ wherein the split ball has a split, the split symmetrical about a second plane.

171. The system according to claim 170_ wherein the split ball has a split, the split symmetrical about a first plane which is non-parallel to a major plane of the paddle assembly.

172. The system according to claim 155_ wherein the means for spreading the first paddle and second paddle apart further comprising a segmented spreadable hinge.

173. The system according to claim 155 wherein the arm has a series of articulations wherein the arm may be bent along a curved arc among a plurality of direction.

174. The system according to claim 173_ wherein the series of articulations are provided through a series of interlocking links.

175. The system according to claim 174_ wherein at least one first link in the series of interlocking links has a first hemispherical surface having a first hemispherical diameter and at least one second link in the series of interlocking links has a second hemispherical indentation having a second hemispherical diameter.

176. The system according to claim 155 wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed on the proximal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.

177. The system according to claim 155 wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed away from the distal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.

178. A system for temporarily immobilizing an area of tissue comprising a paddle assembly, paddle assembly having a first paddle and a second paddle, the paddle assembly further having means for moving the first paddle relative to the second paddle; an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm having means for permitting the arm to flex, the arm having means for fixing the arm to an object; and arm locking means coupled to the arm, the arm locking means permitting the locking of the arm in any selected position wherein the distal end of the arm is maintained in the selected position.

179. The system according to claim 178__ wherein the means for moving the first paddle relative to the second paddle further comprise means for spreading the first paddle away from the second paddle.

180. The system according to claim 179_ wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed on the proximal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.

181. The system according to claim 180_ wherein the spreading actuator is a torque screw.

182. The system according to claim 178 wherein the first paddle has means for engaging heart tissue.

183. The system according to claim 182 wherein the means for engaging heart tissue further comprises at least a first suction port positioned along a first surface of the first paddle.

184. The system according to claim 183 wherein the means for engaging heart tissue further comprises at least a second suction port positioned along a second surface of the second paddle.

185. The system according to claim 185 wherein the first surface and the second surface are generally within the same plane.

186. The system according to claim 184 further comprising the first paddle is adapted to have a first surface which conforms to the surface of the heart.

This is an alternative claim NOT HAVING flexible but still having arm spreading.

187. A system for stabilizing tissue comprising
a paddle assembly, paddle assembly having a first paddle and a second paddle. the paddle assembly
further having means for spreading the first paddle away from the second paddle;
an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm
having means for fixing the arm to an object; and
means for spreading the first paddle and second paddle apart, the means for spreading coupled to a
proximal end of the arm.

188. The system according to claim 187_ wherein the first paddle has a first surface, a first suction
port positioned within the first surface, a second suction port positioned within the first surface, a third
suction port positioned within the first surface

189. The system according to claim 188_ wherein the first suction port, the second suction port, and
the third suction port are all in a linear relation.

190. The system according to claim 187_ wherein the means for spreading further comprise means
for independently spreading the first paddle and second paddle apart.

191. The system according to claim 187_ wherein the means for spreading the first paddle away
from the second paddle further comprising means for spreading the first paddle away from the second
paddle a parallel relation.

192. The system according to claim 187_ wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle in a non parallel relation.

193. The system according to claim 187 wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge.

194. The system according to claim 187_ wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart

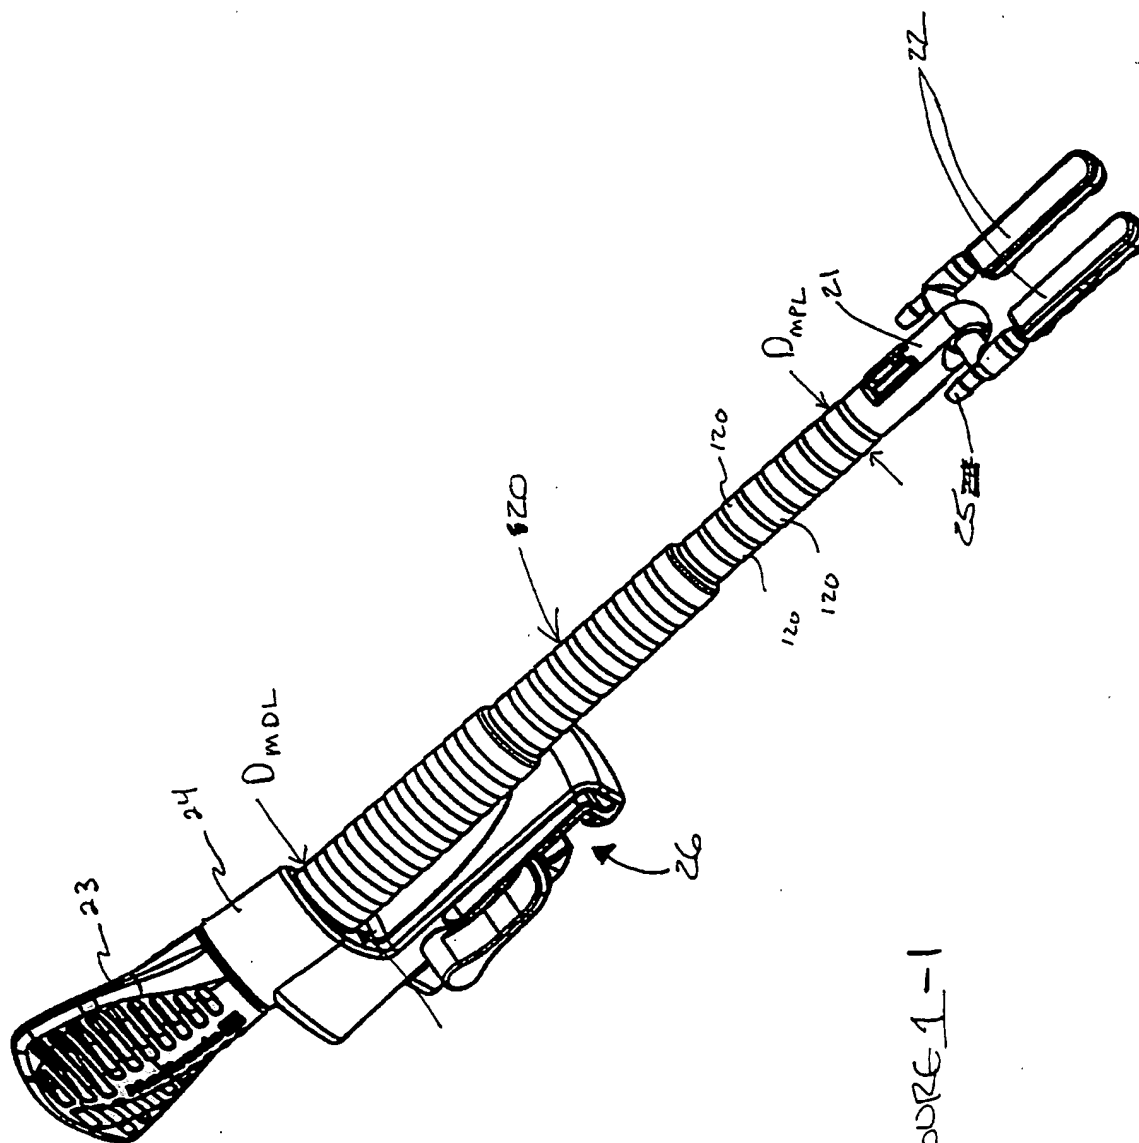


FIGURE 1-1

FIG 1-2

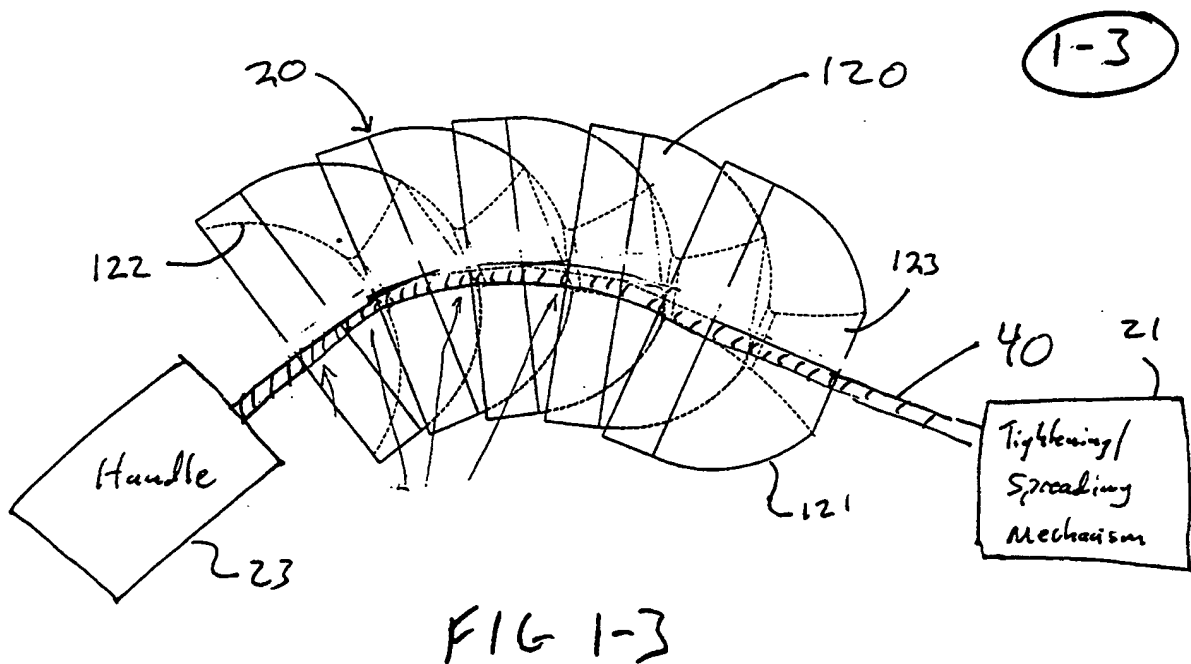
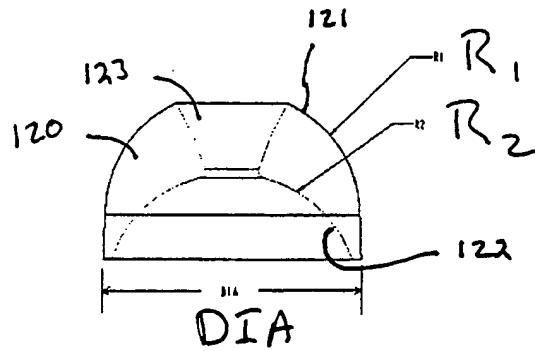


FIG 1-3

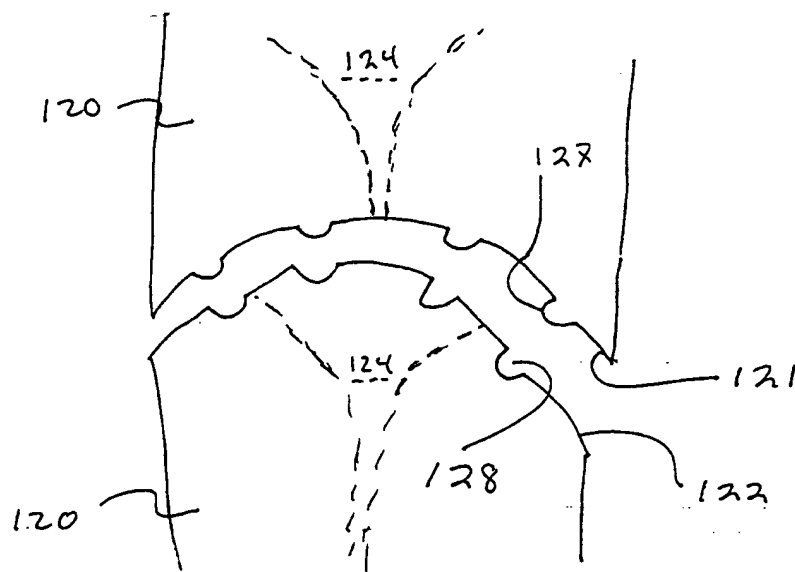


Fig 1-5

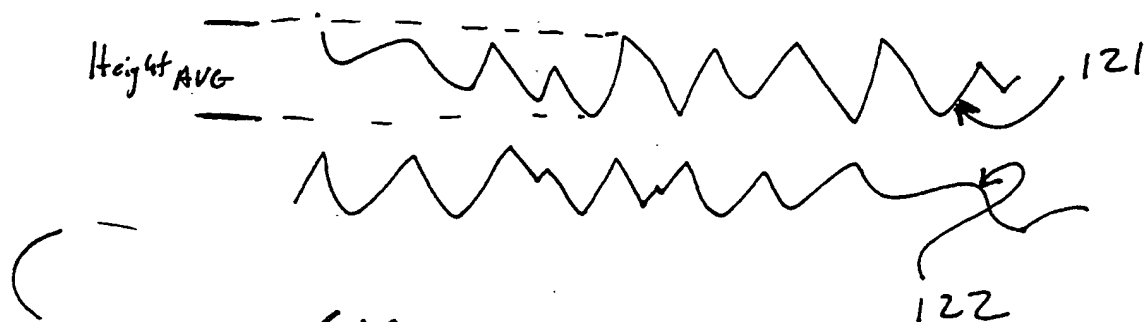


FIG 1-4

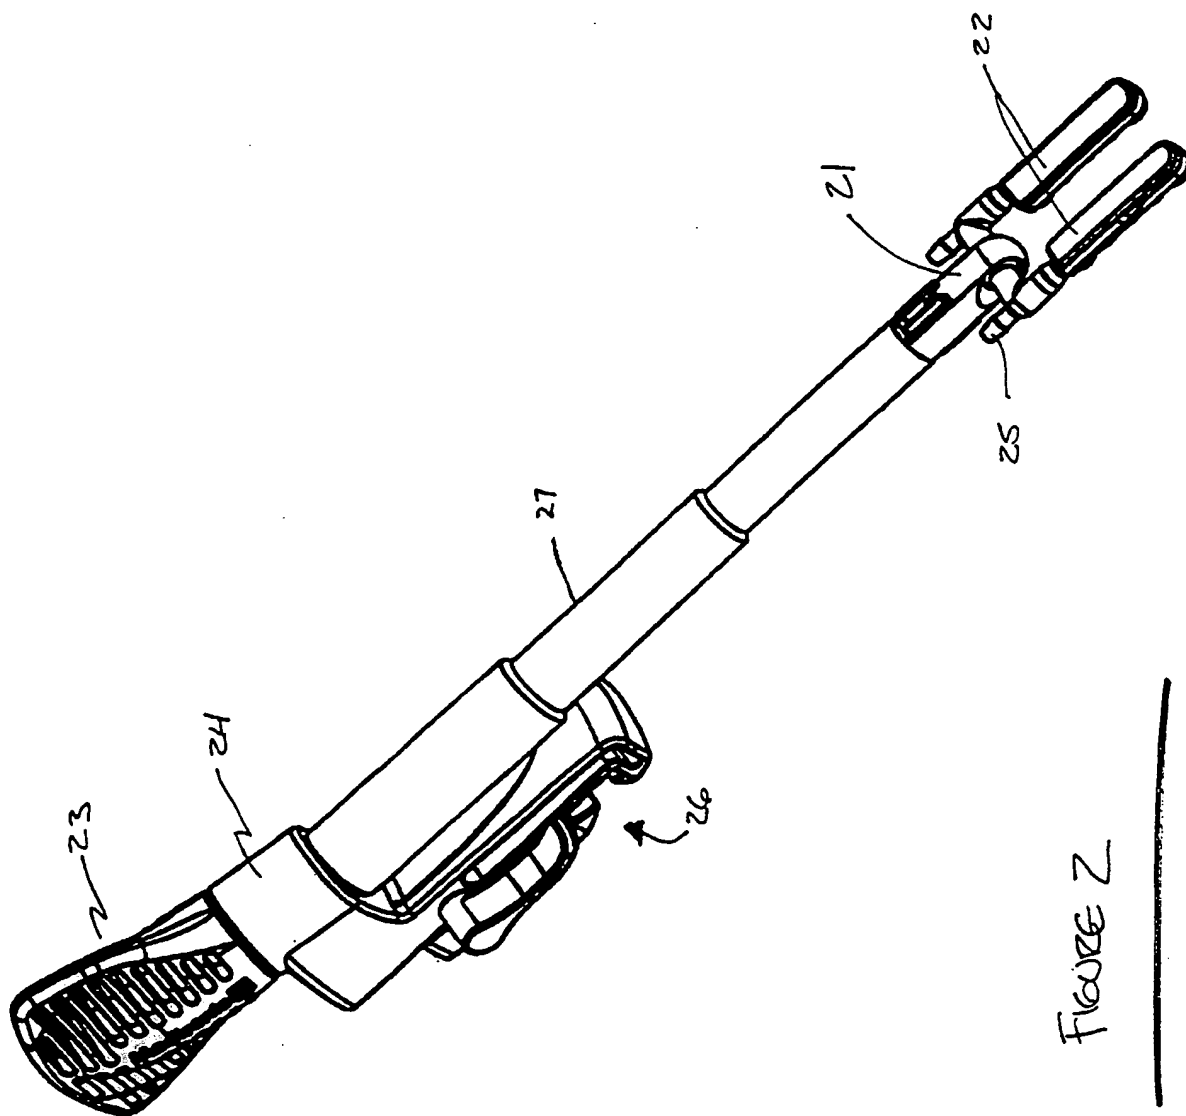


FIGURE 2

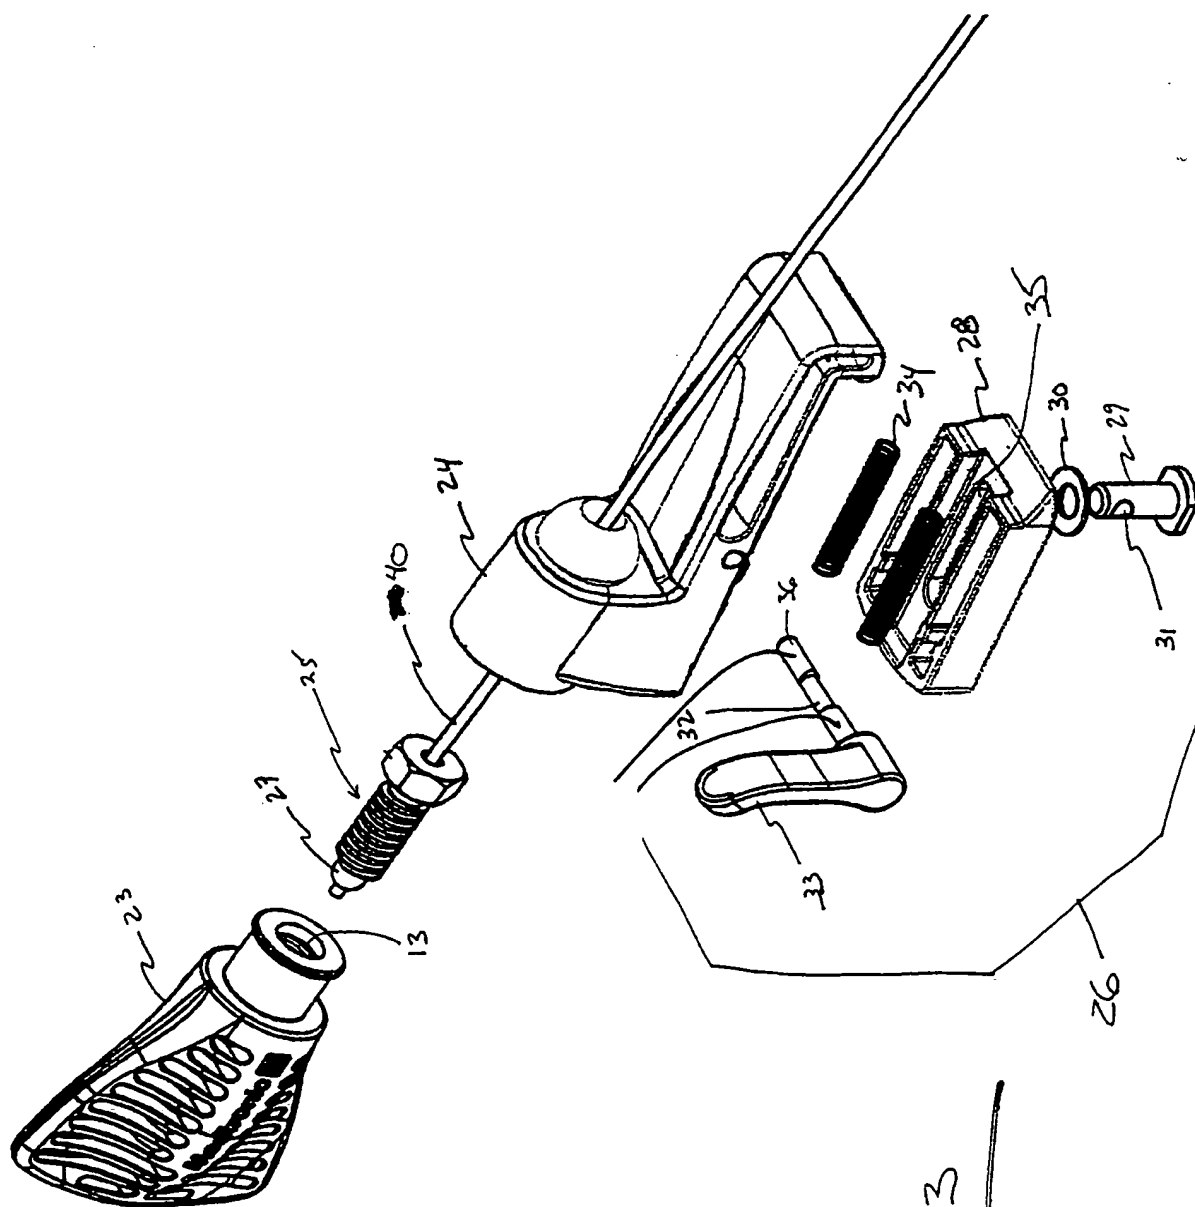


FIGURE 3

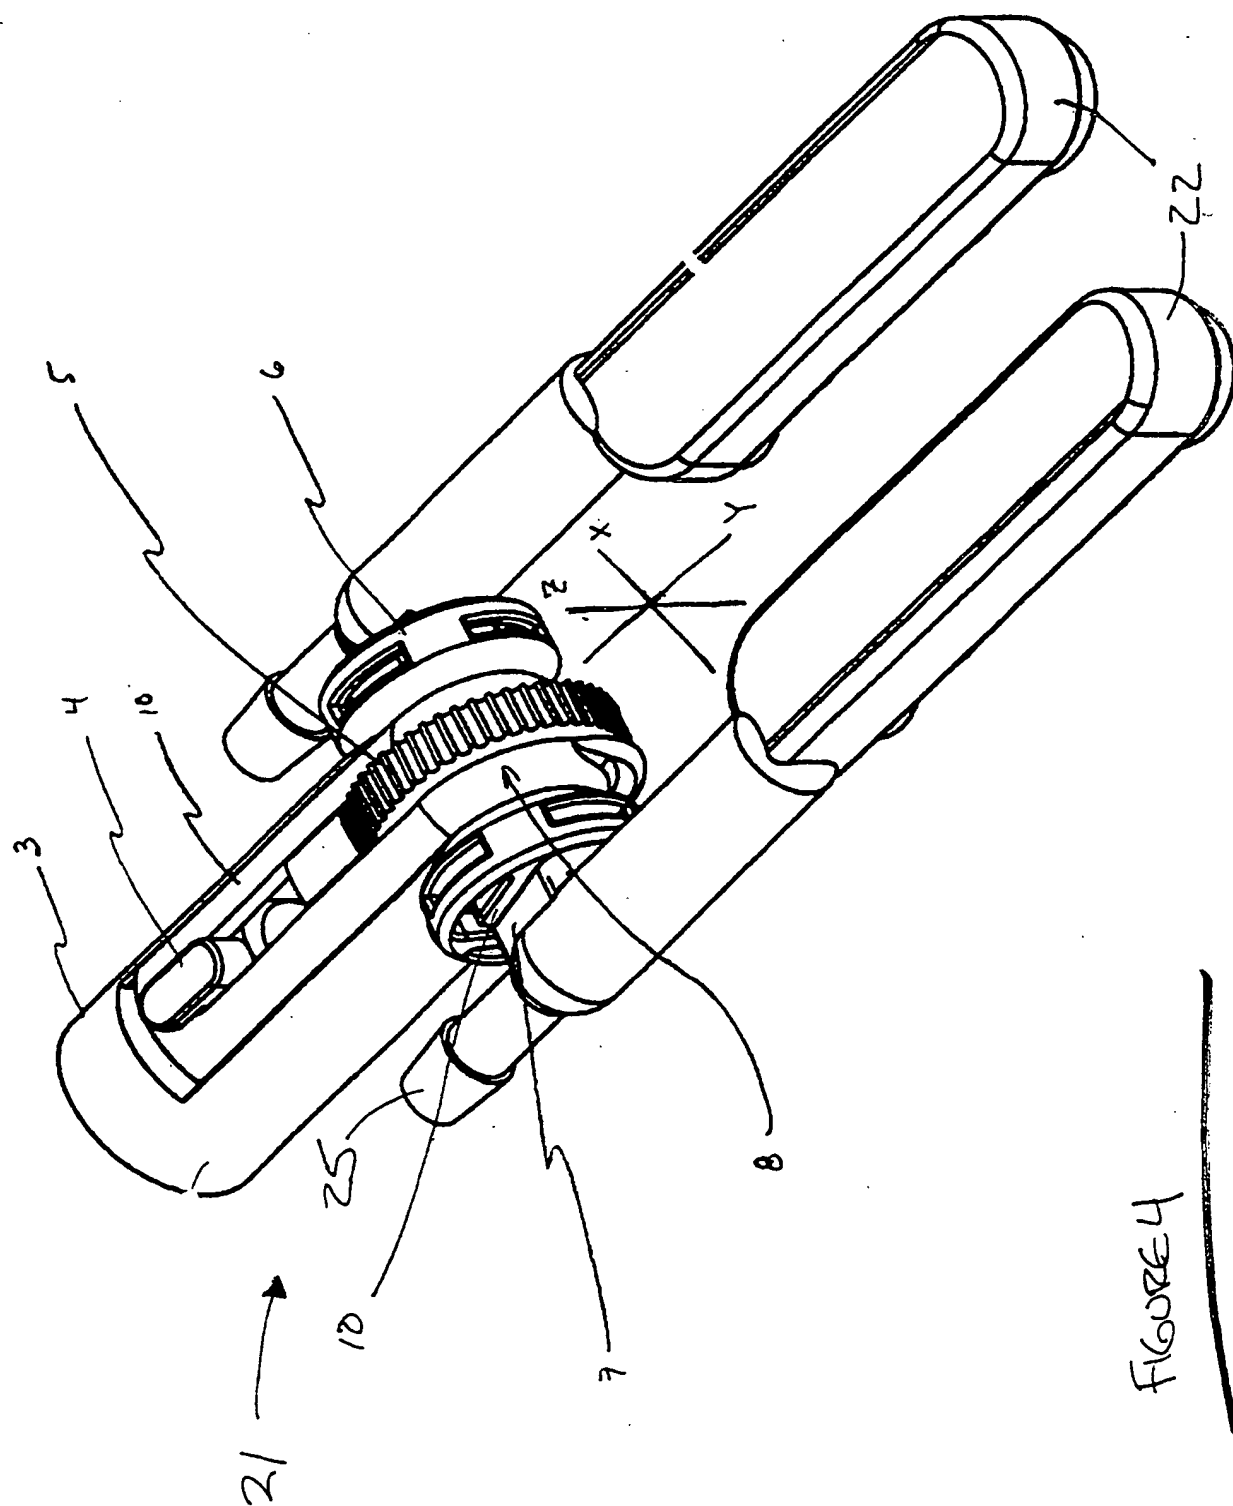


FIGURE 4

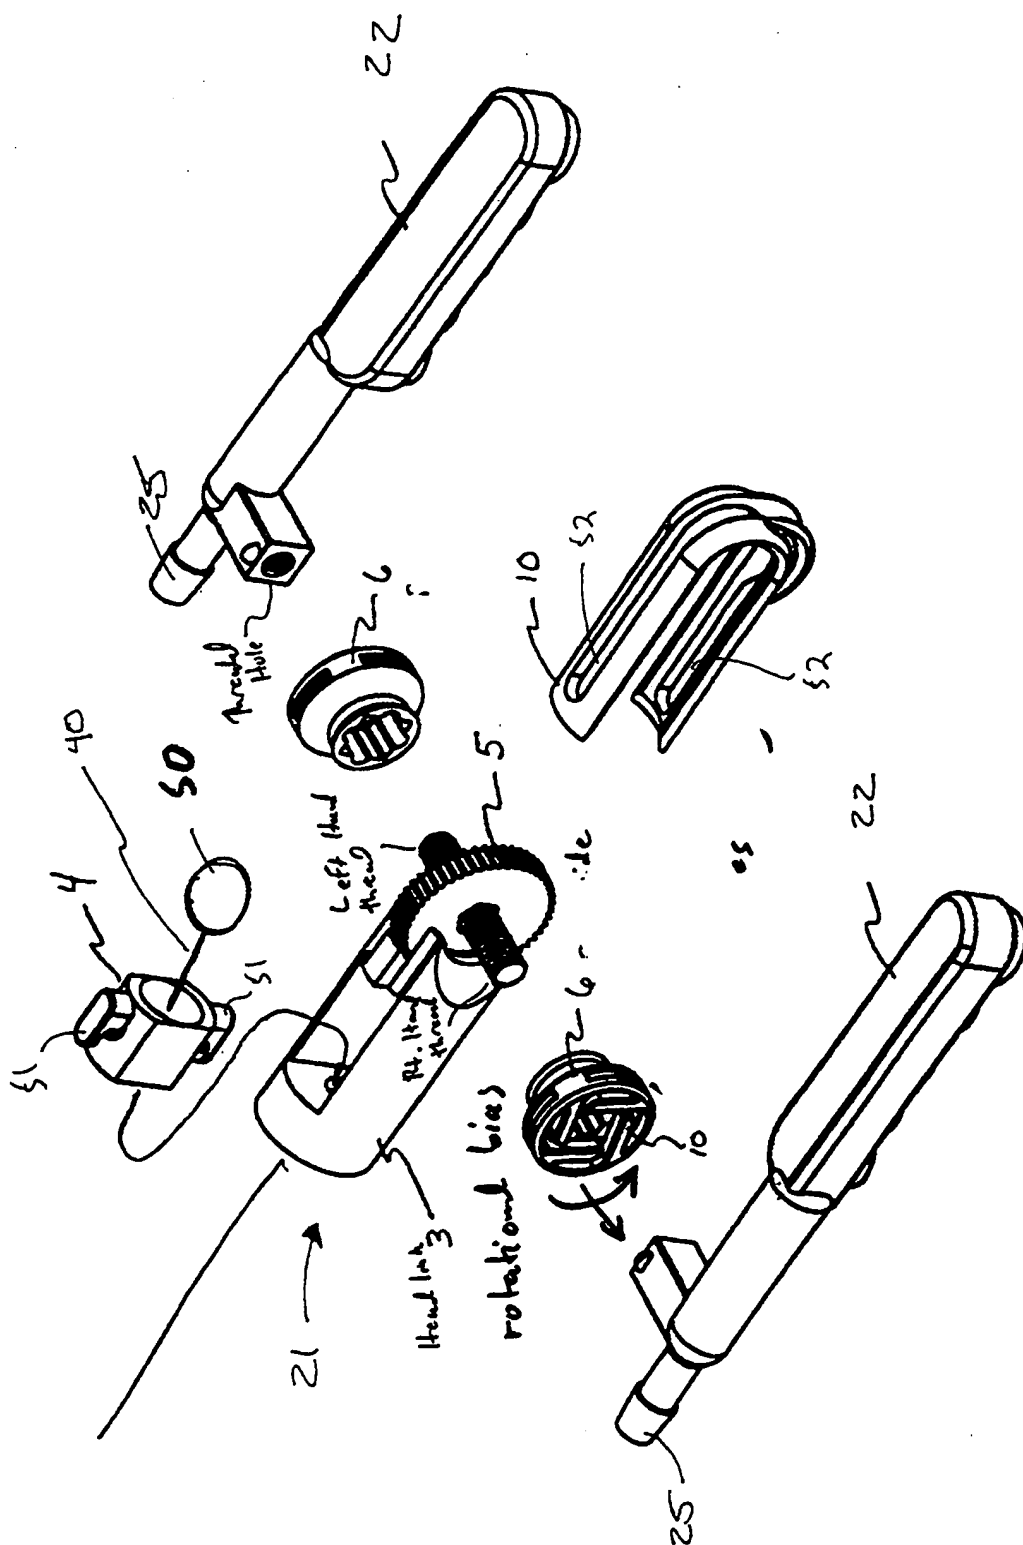


Figure 5

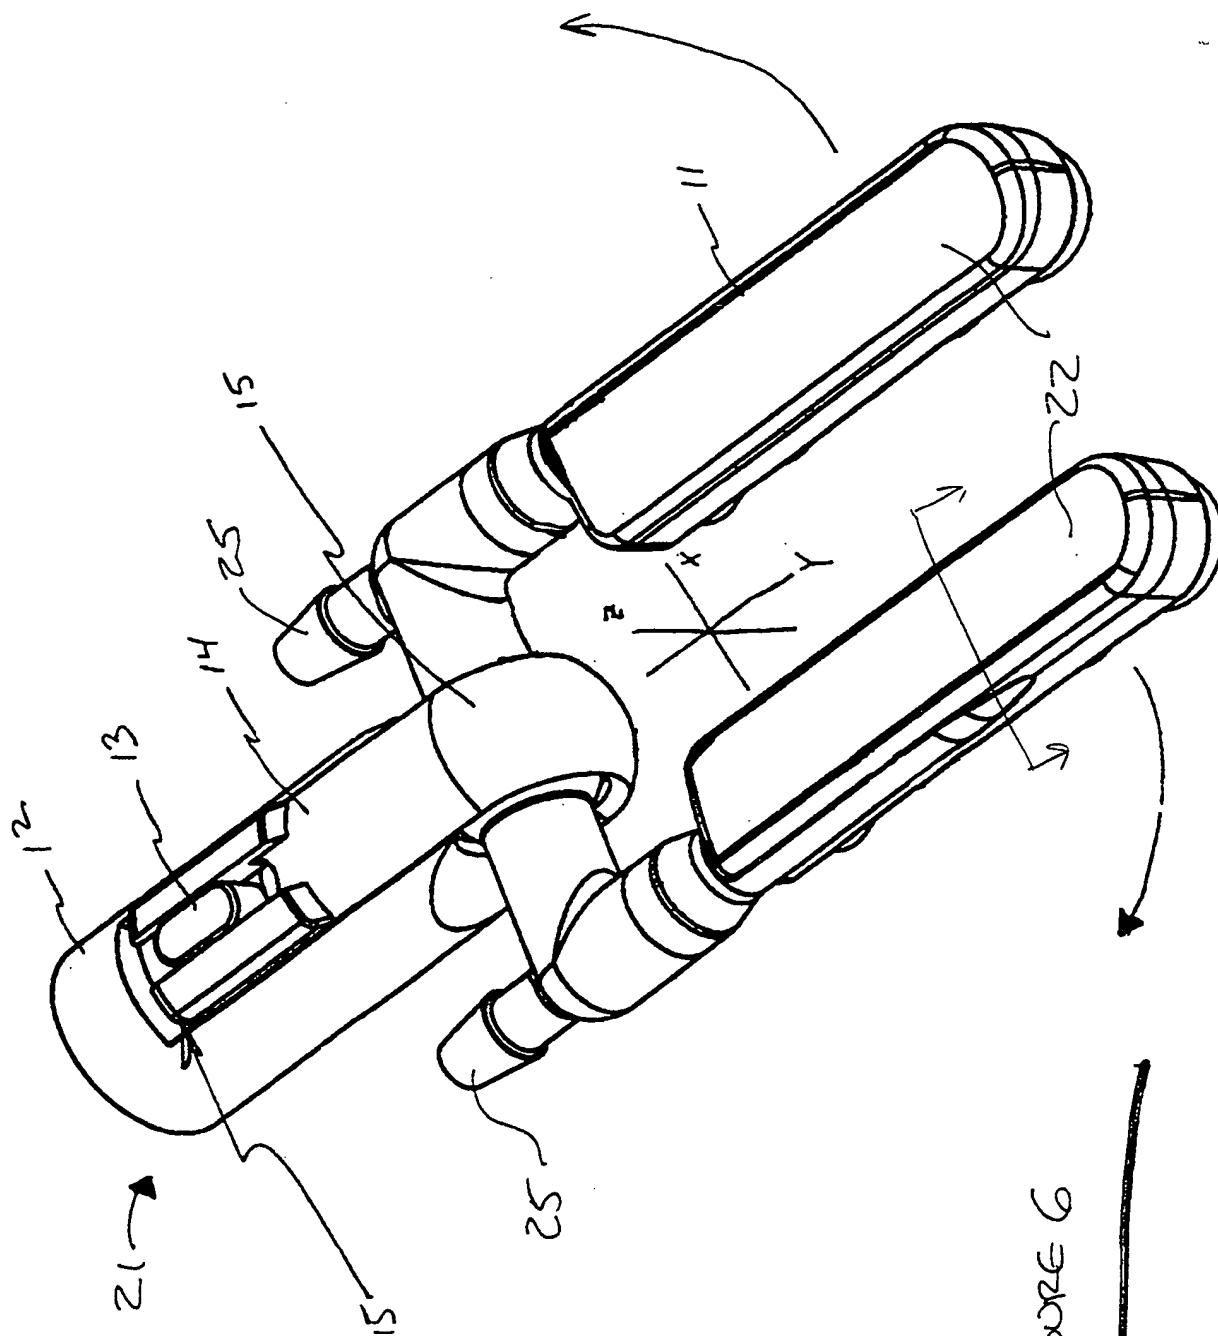
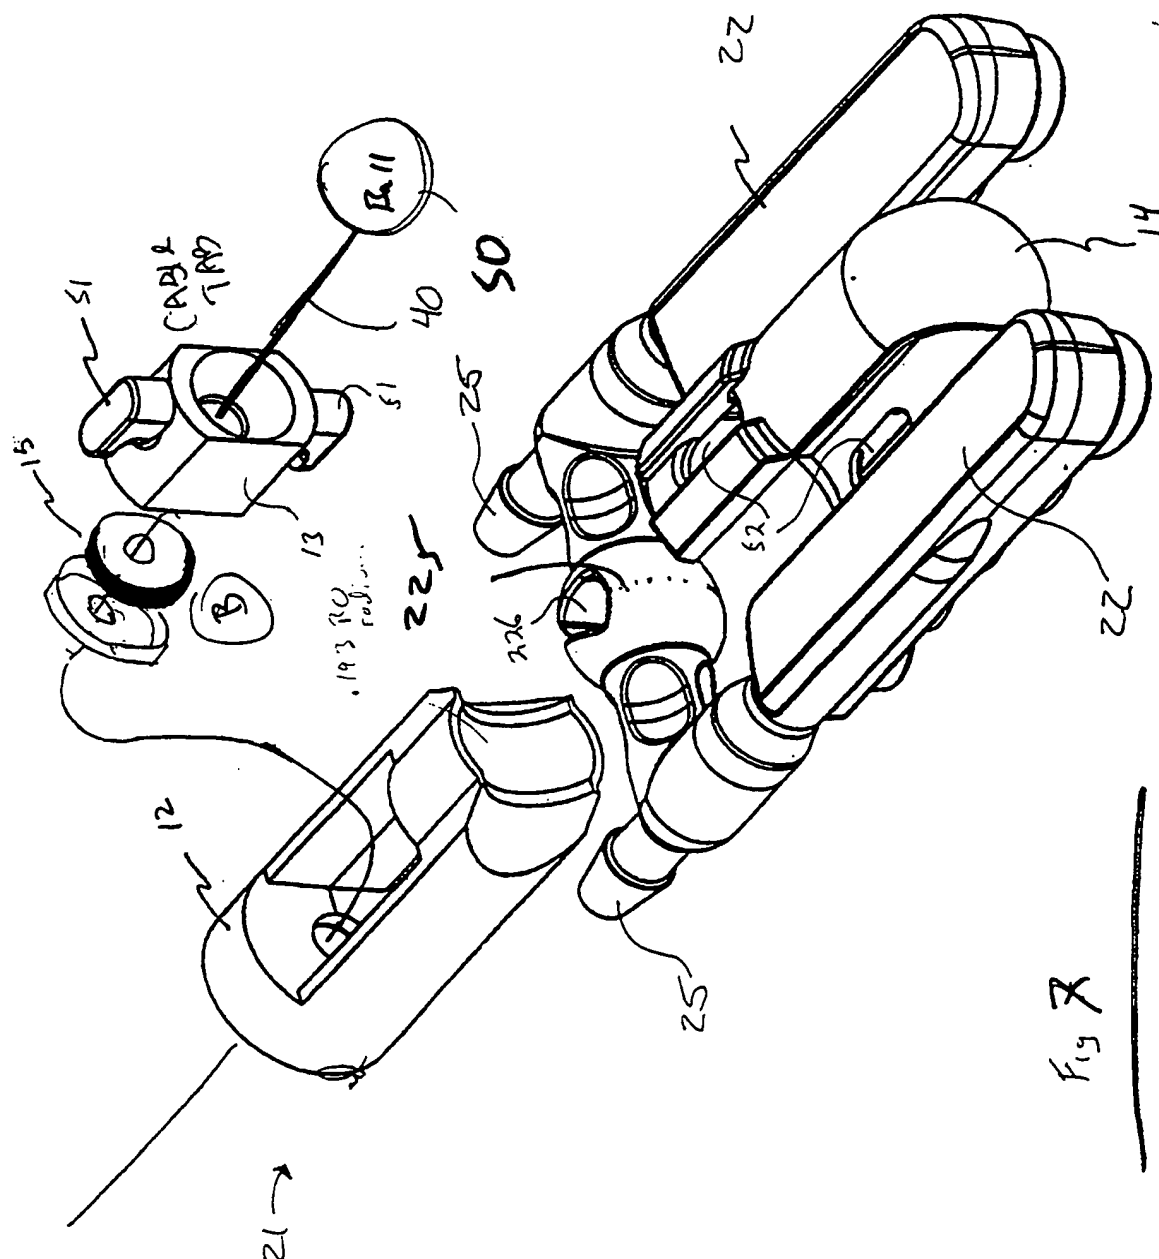


FIGURE 6



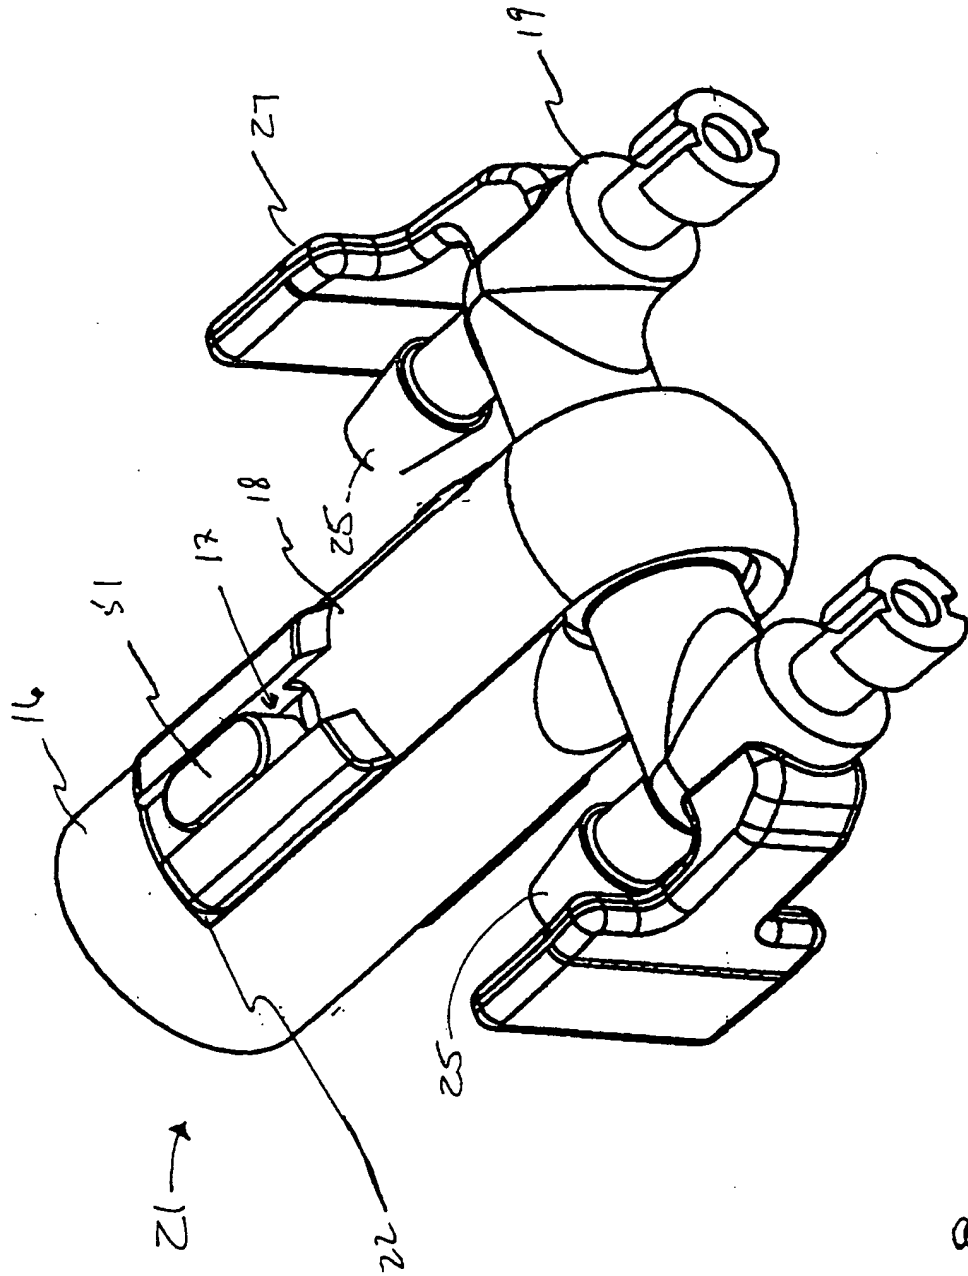


FIGURE 8

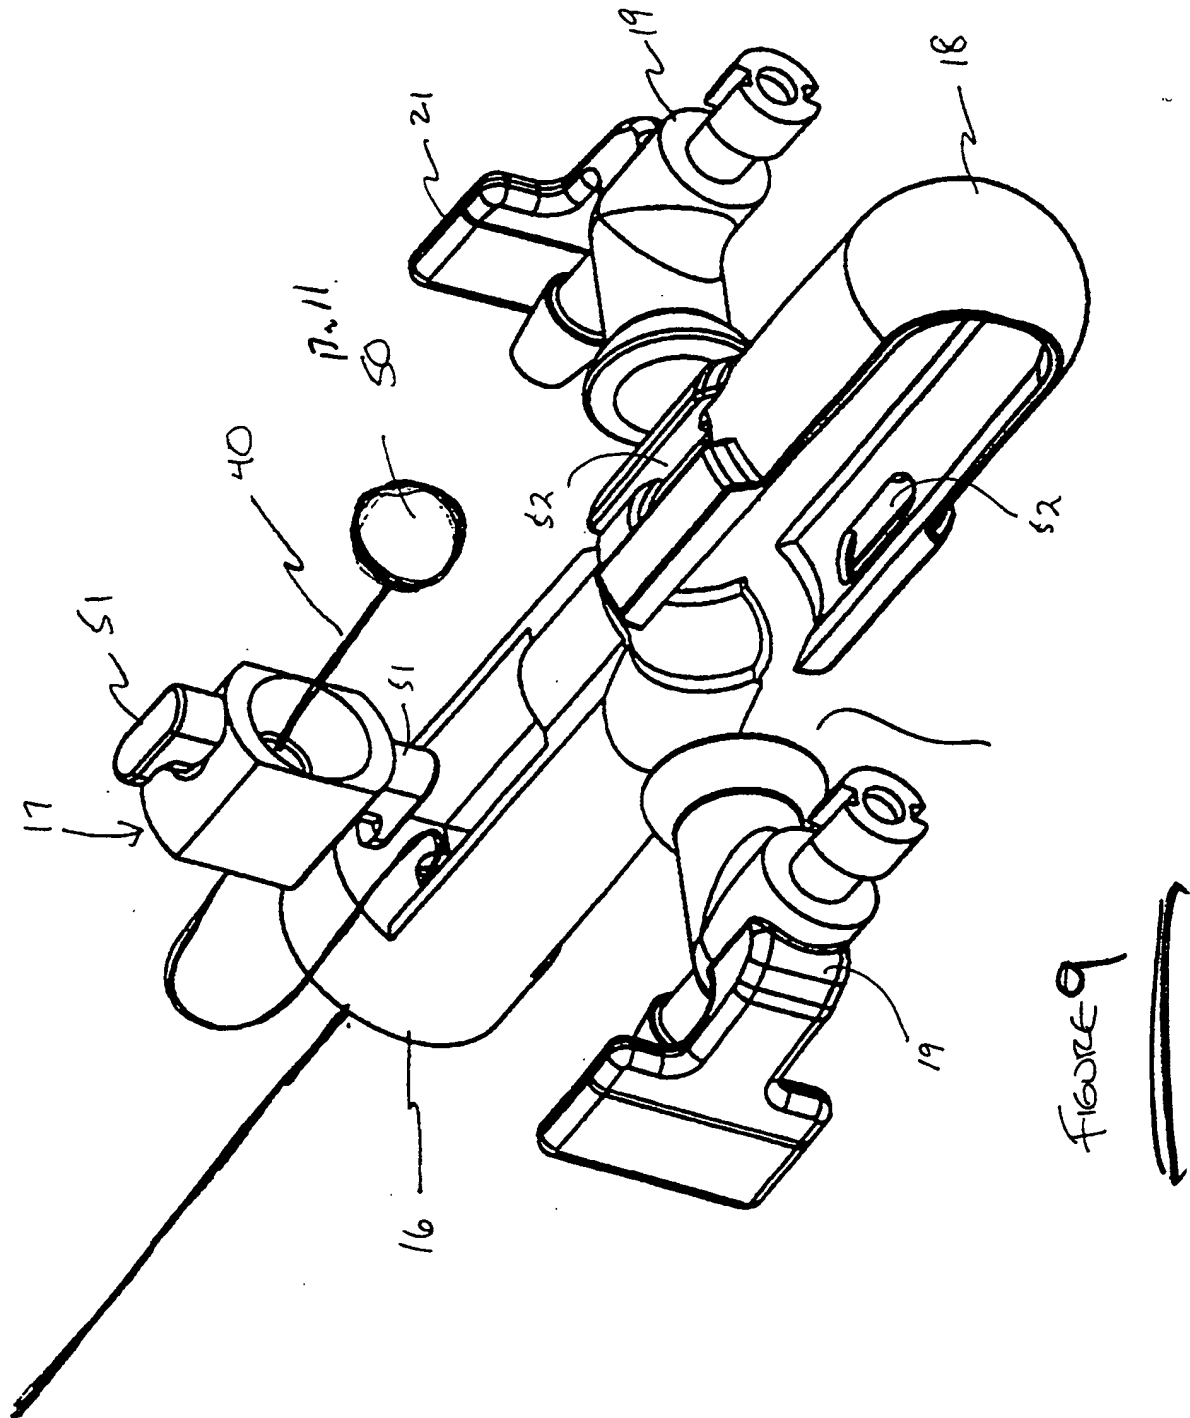


Figure 9

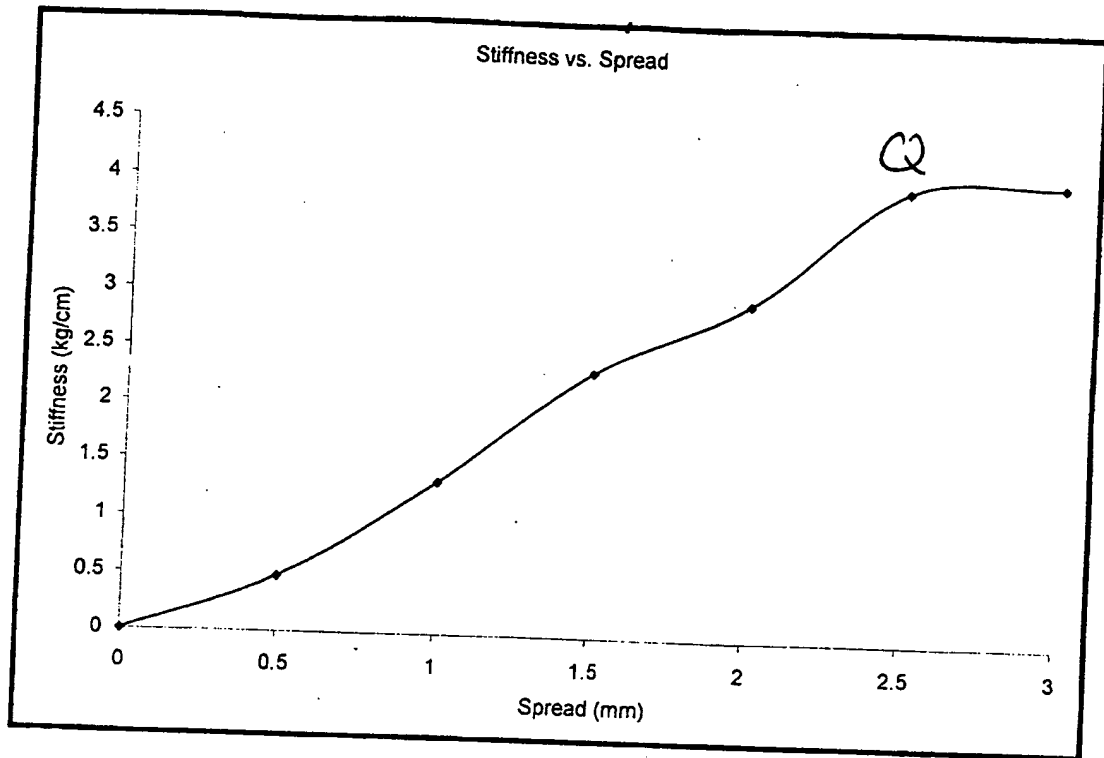


FIG 10

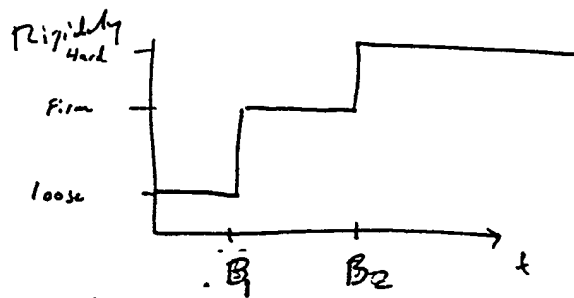


Fig 11

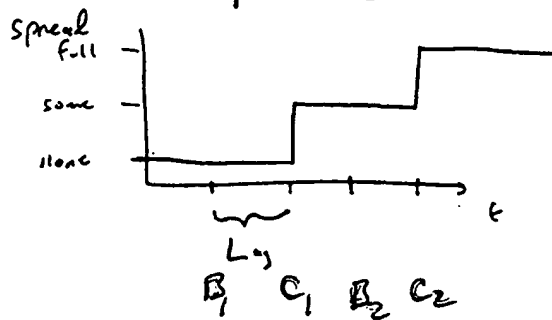
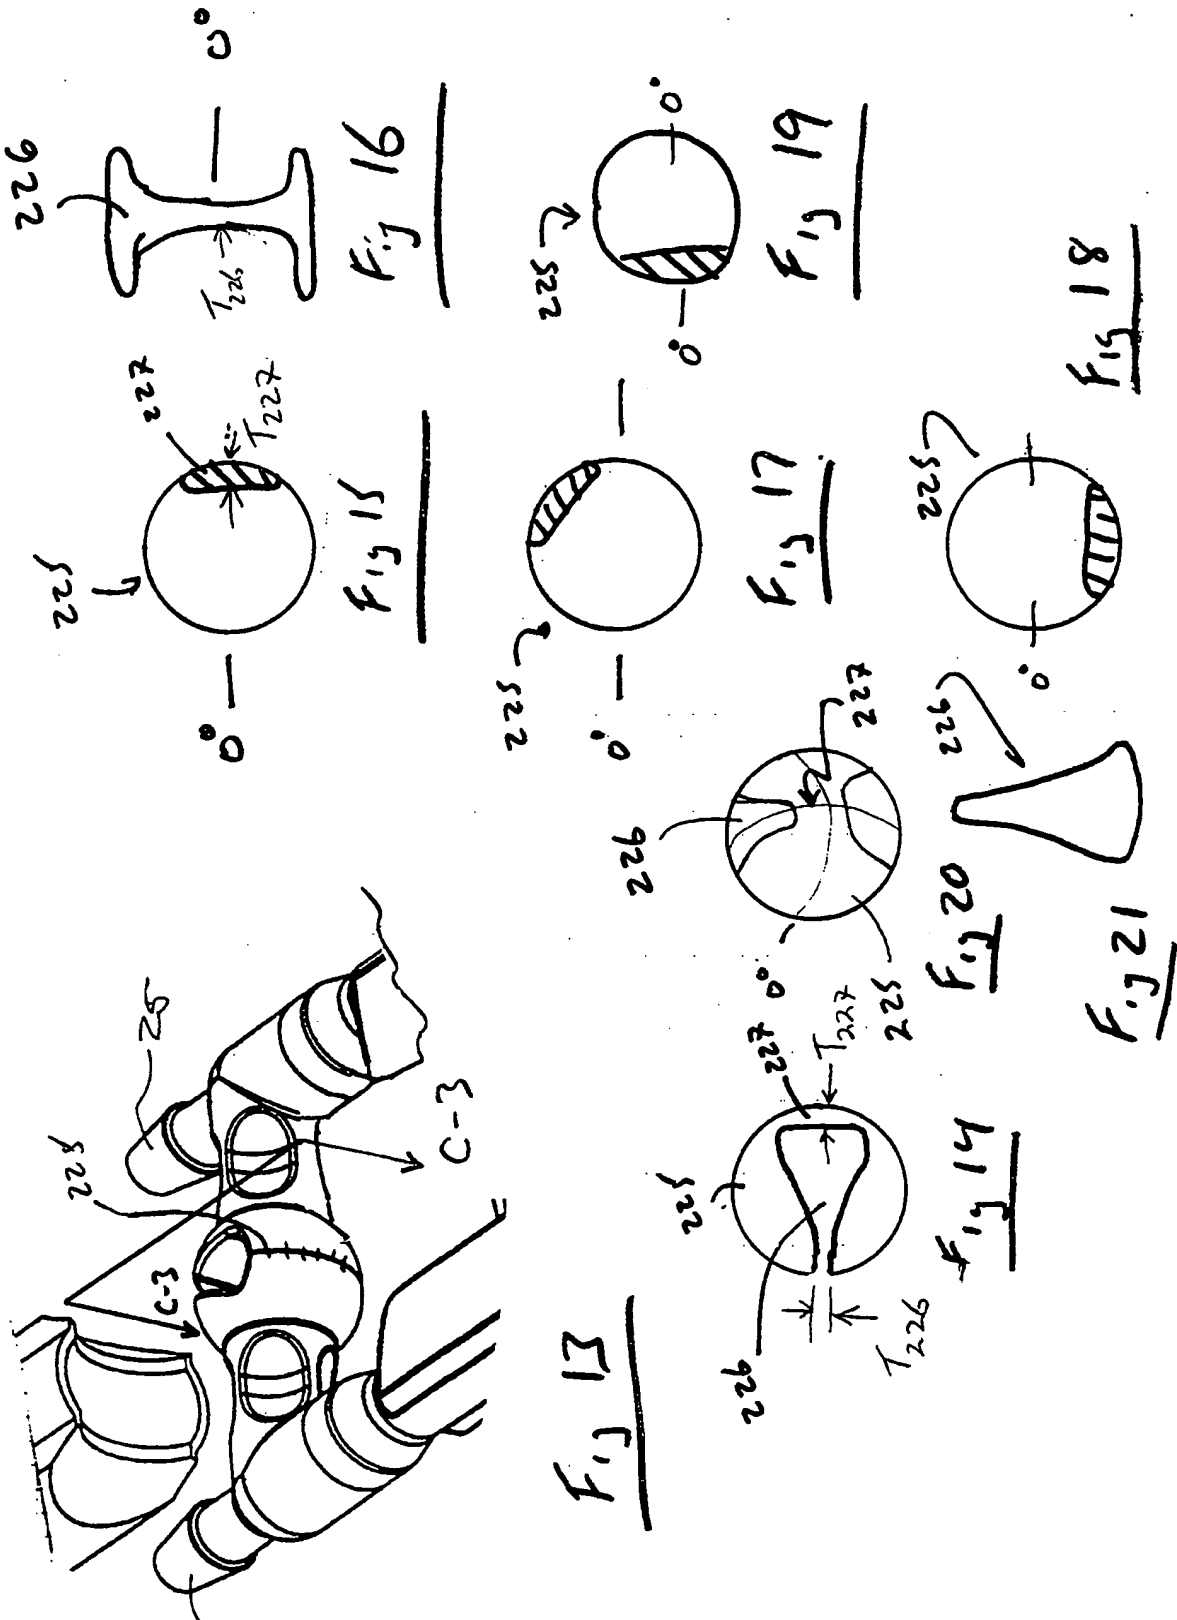


Fig 12






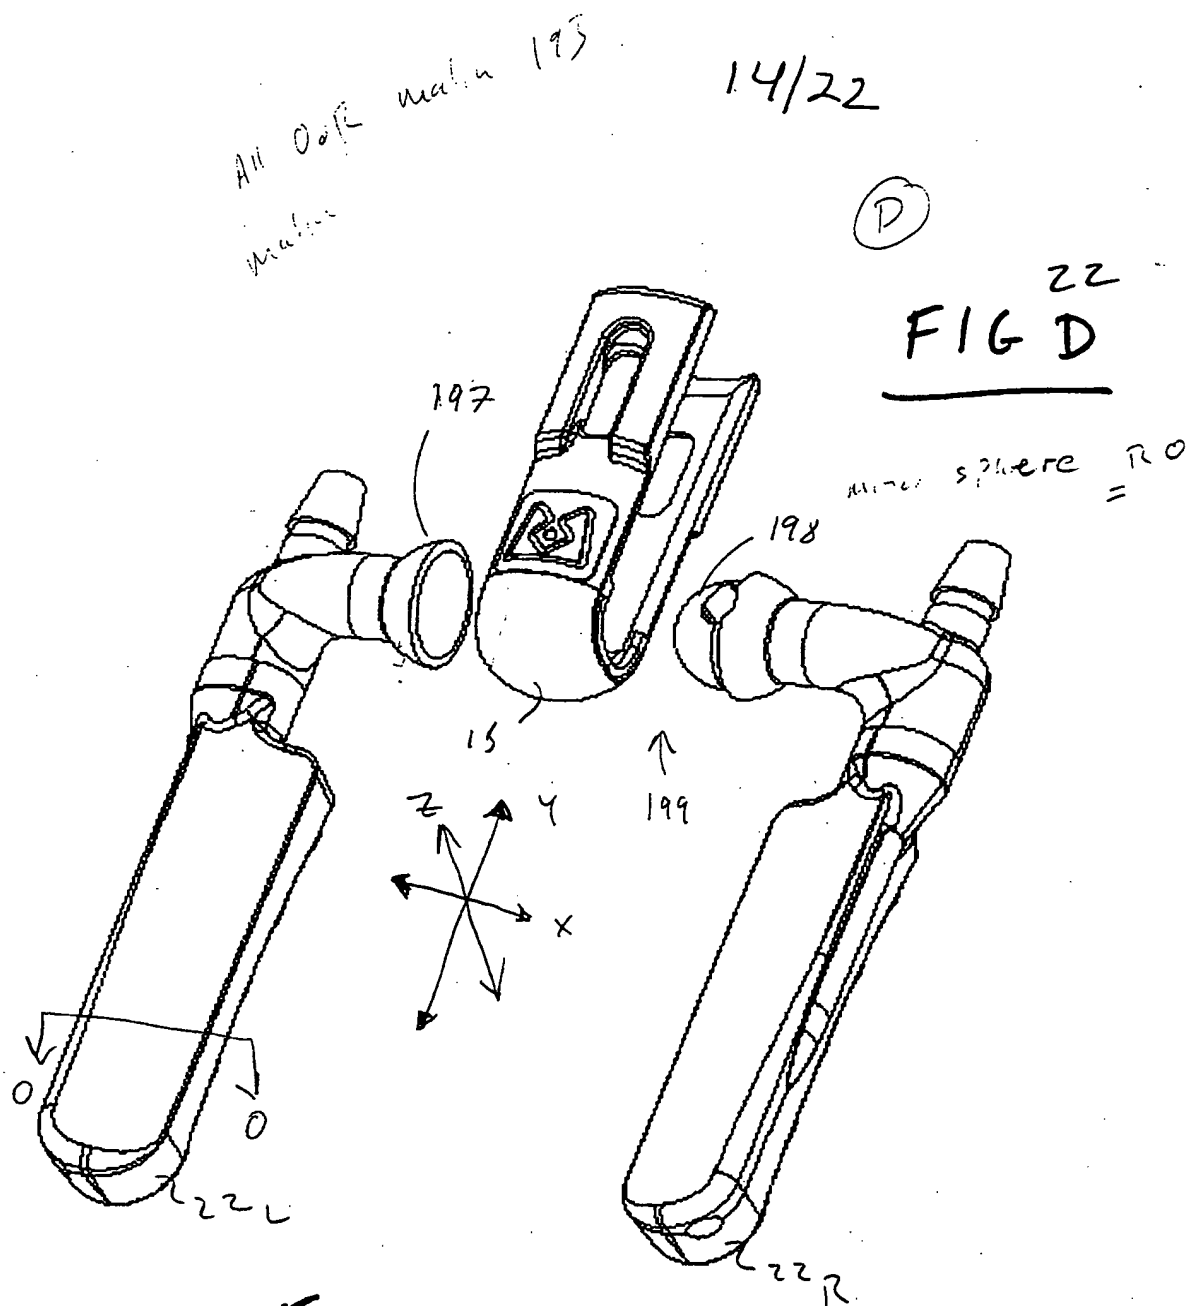


Fig 22



" Segmented spreadable hinge Flaring Paddle

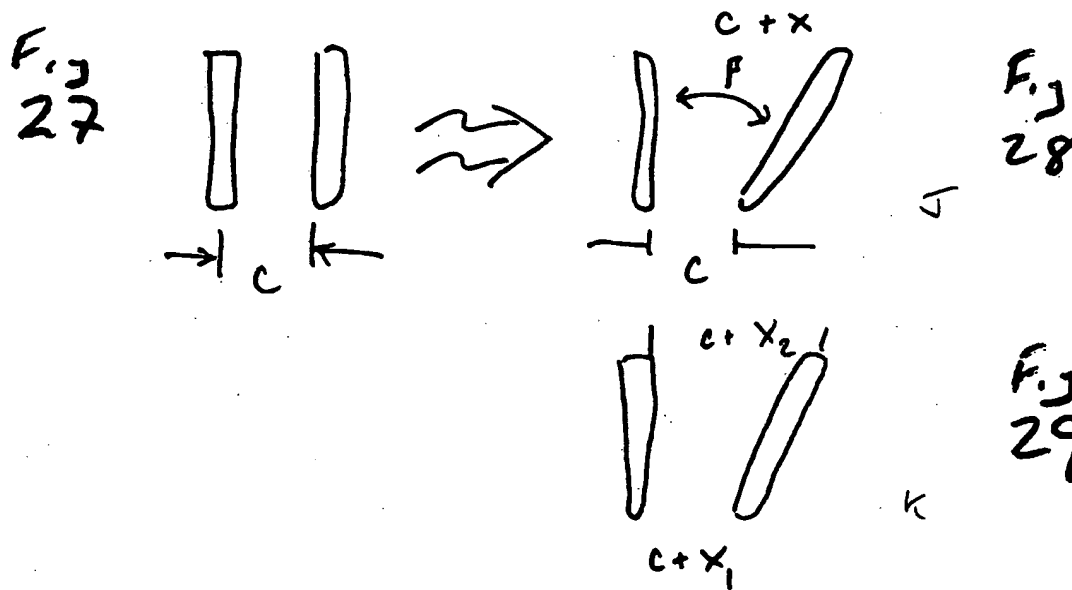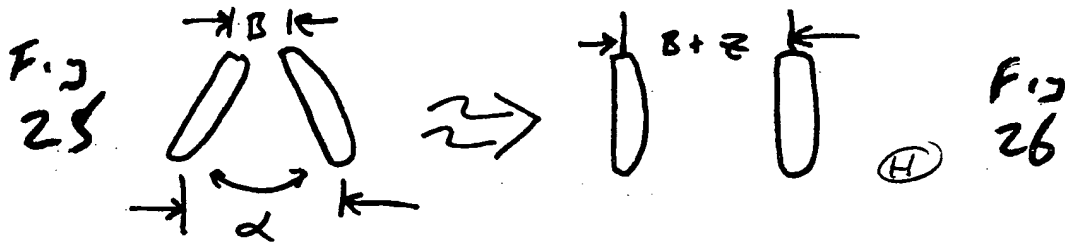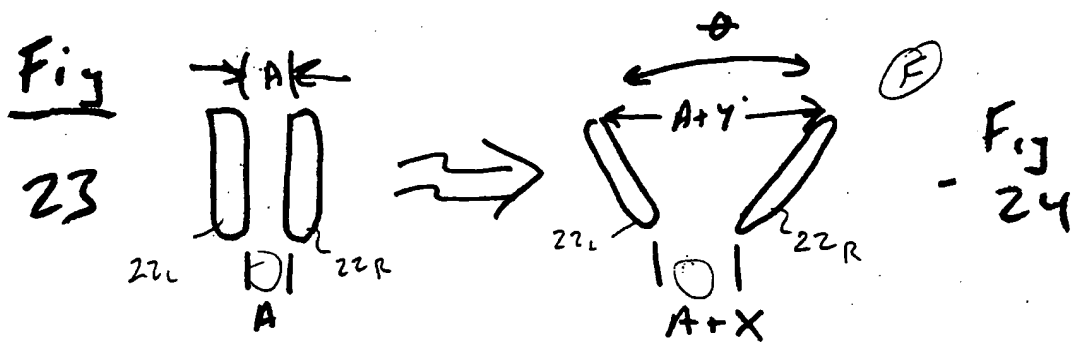


— Fig D or Thum's wheel

— add only one
screw threaded
So only one ped screw

see
Figs 4 & 5

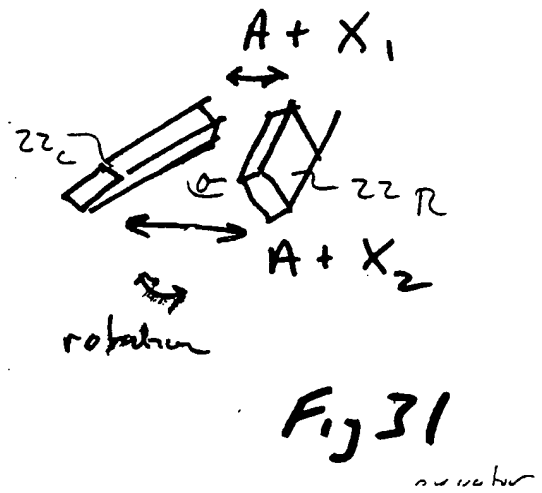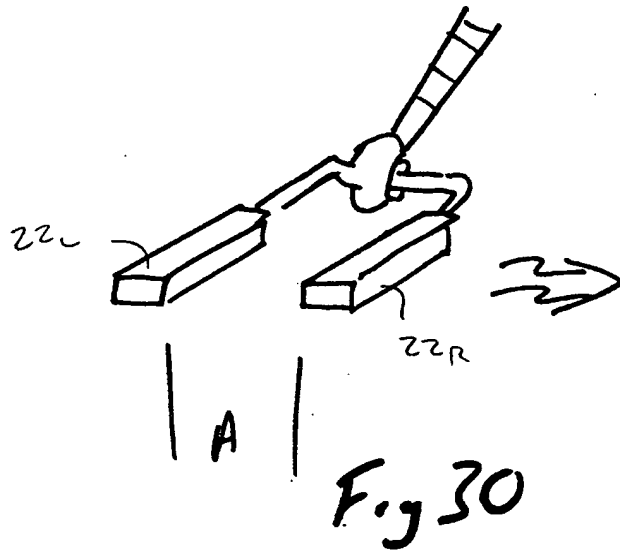

77

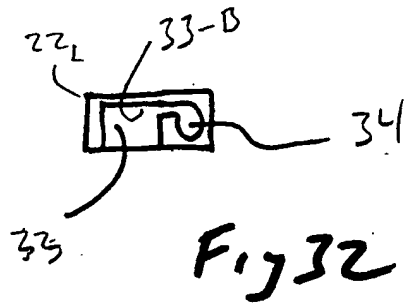

$$\frac{\downarrow}{H} \frac{1}{r}$$

3 - zaman in p₂

70

14g

Fig
33

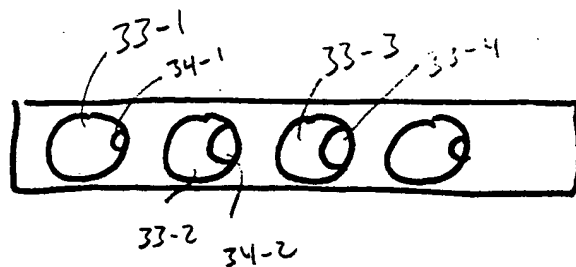


Fig
34

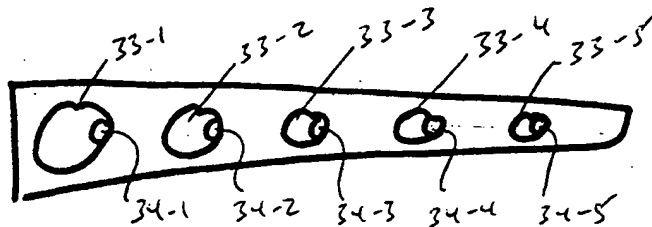


Fig
35

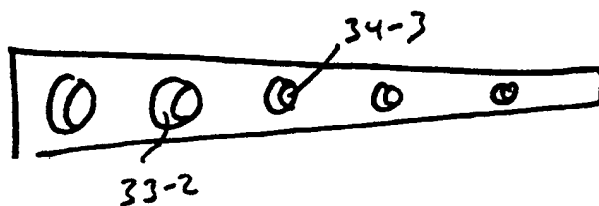


Fig
36

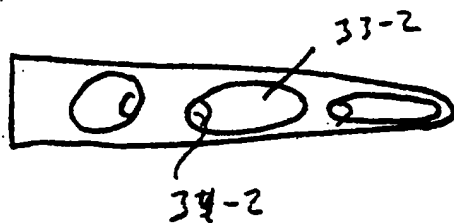


Fig
37

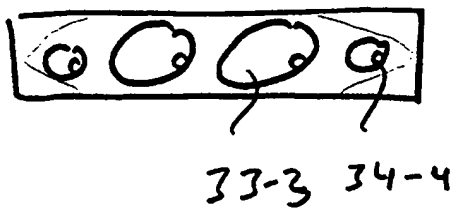


Fig 38

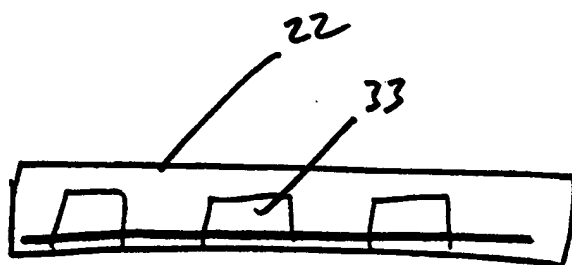
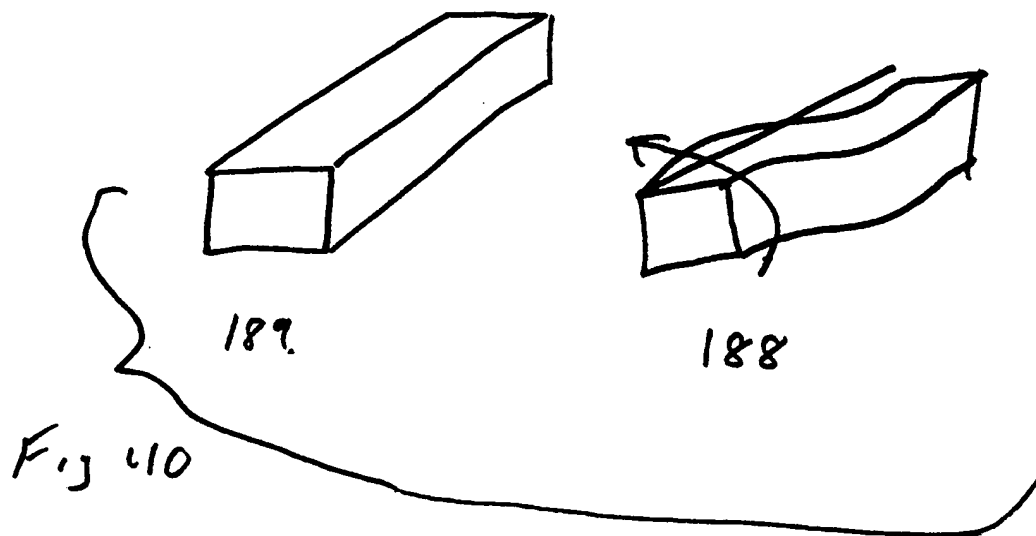
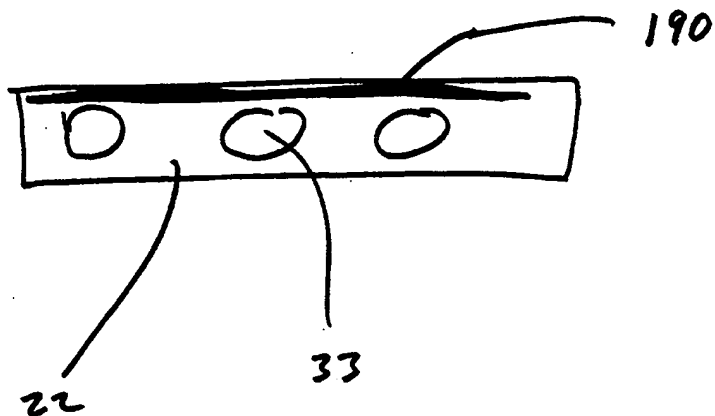


Fig 39



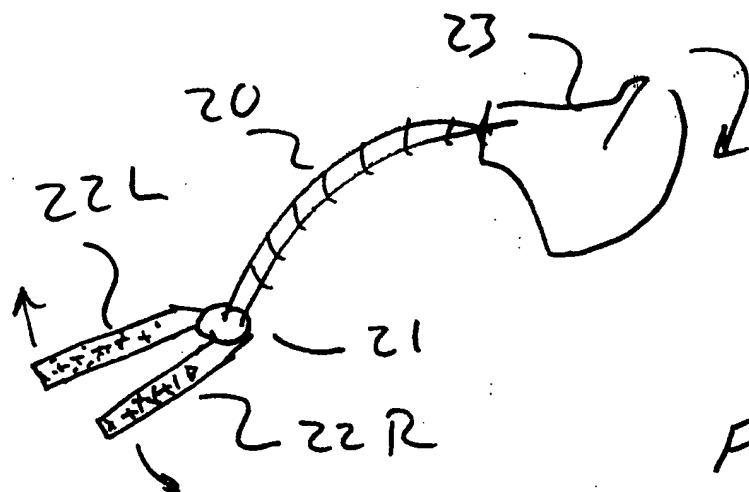


Fig 41

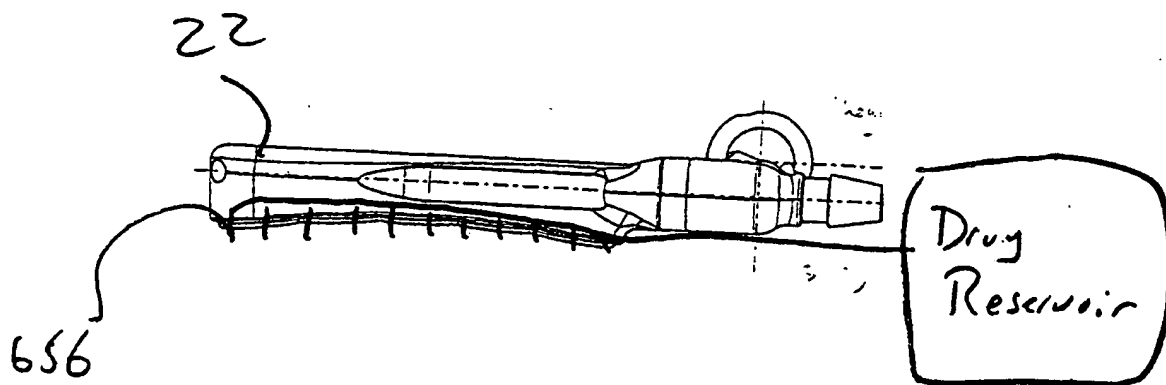


Fig 42

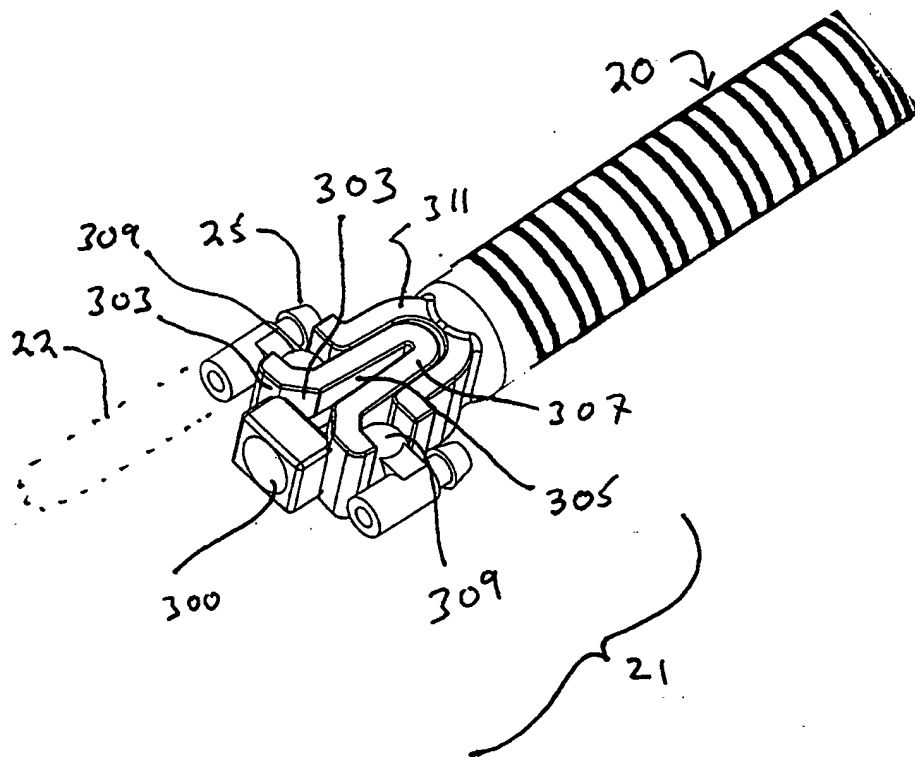


Fig 43


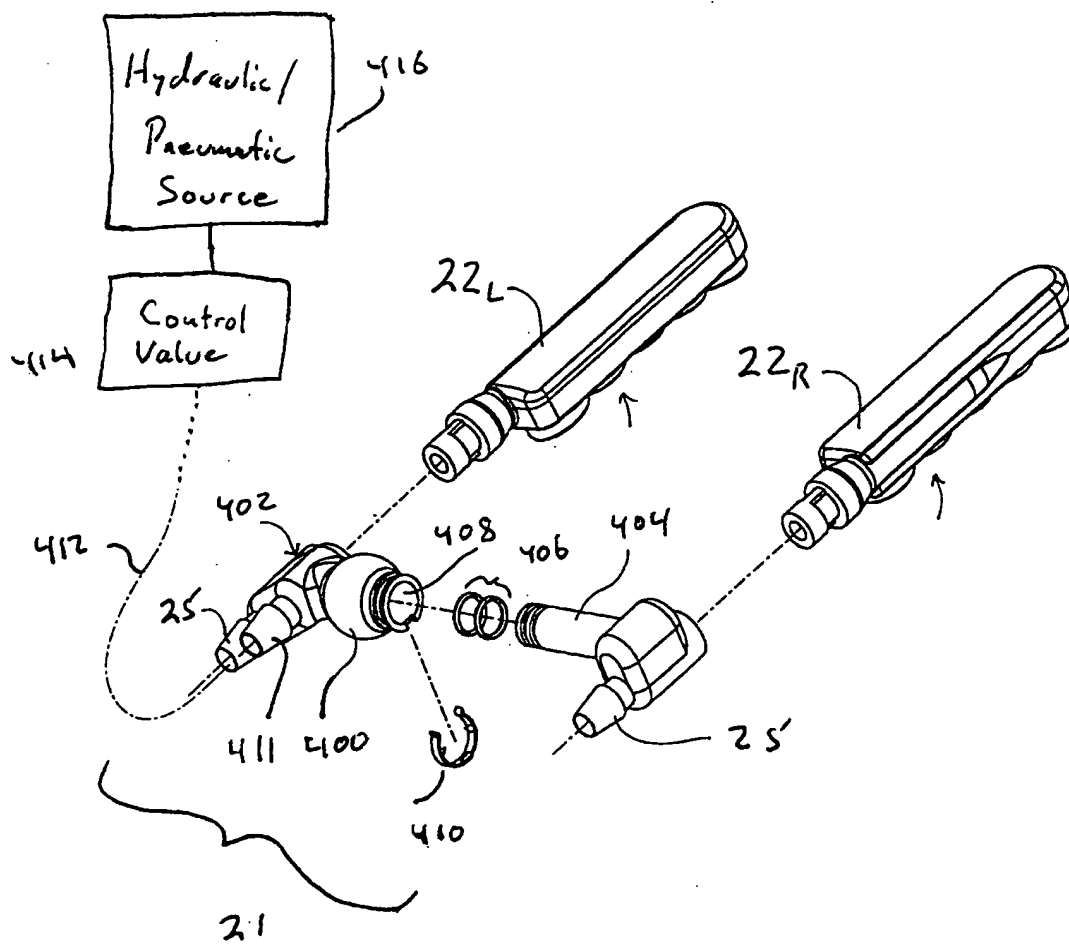


Fig 44

Fig 45



(19) World Intellectual Property Organization
International Bureau

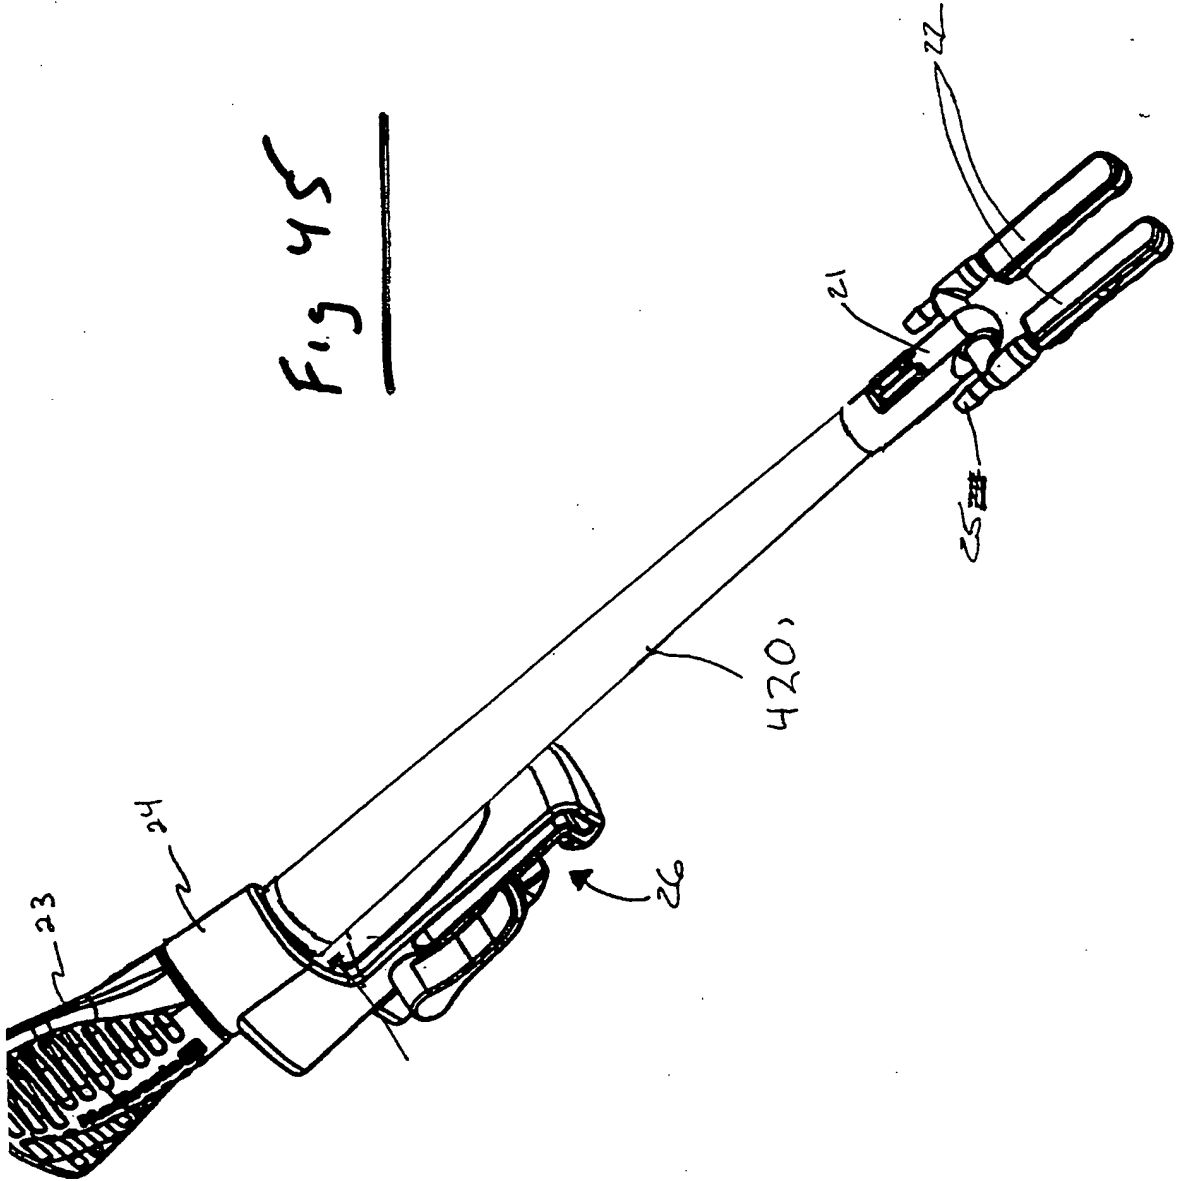

(43) International Publication Date
23 March 2000 (23.03.2000)


PCT

(10) International Publication Number
WO 00/15119 A3




- (51) International Patent Classification⁷: **A61B 17/02**
- (21) International Application Number: **PCT/US99/20305**
- (22) International Filing Date:
3 September 1999 (03.09.1999)
- (25) Filing Language: **English**
- (26) Publication Language: **English**
- (30) Priority Data:
60/100,443 15 September 1998 (15.09.1998) **US**
- (63) Related by continuation (CON) or continuation-in-part (CIP) to earlier application:
US 60/100,442 (CIP)
Filed on 15 September 1998 (15.09.1998)
- (71) Applicant (for all designated States except US): **MEDTRONIC, INC.** [US/US]; 7000 Central Avenue NE, Minneapolis, MN 55432 (US).
- (72) Inventors; and
(75) Inventors/Applicants (for US only): **BORST, Cornelius** [NL/NL]; Obrechtlaan 55, NL-3723 KB Bilthoven (NL). **MANSVELT-BECK, Hendricus, J.** [NL/NL]; Bildzigt 14, NL-3721 KK Bilthoven (NL). **BOONE, Eric** [US/US]; 7258 Walnut Avenue, Jenison, MI 49428 (US). **GOODMAN, Jack** [US/US]; 3228 Cottontail Court, Ann Arbor, MI 48103 (US). **HALL, John, D.** [US/US]; 2957 Longstreet Avenue SW, Wyoming, MI 49509 (US). **O'NEILL, William, G.** [US/US]; 7267 Cuesta Way Drive, Rockford, MI 49341 (US). **TESTA, Vincent, J.** [US/US]; 510 North Center Drive, Grand Rapids, MI 49544 (US). **VROEGOP, Eric** [US/US]; 105 Birchwood, Holland, MI 49423 (US).
- (74) Agents: **JARO, Michael, J. et al.**; Medtronic, Inc. MS301, 7000 Central Avenue N.E., Minneapolis, MN 55432 (US).
- (81) Designated States (national): **AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP,**

[Continued on next page]

(54) Title: **METHOD AND APPARATUS FOR TEMPORARILY IMMOBILIZING A LOCAL AREA OF TISSUE**

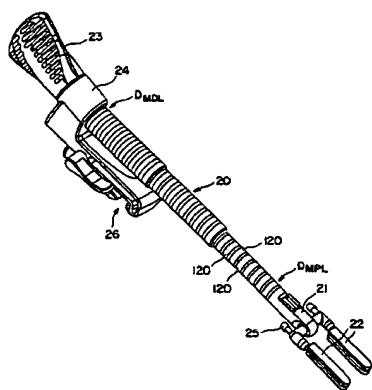

(57) Abstract: The invention is a method and apparatus for performing beating heart surgery, in which a single articulating arm supports multiple suction pods. Once the suction pods are applied to the heart surface, tightening a cable fixes the arm in place. Then, the suction pods may be spread apart from each other to tighten the surface of the cardiac tissue lying between the suction pods. In one embodiment, fixation of the arm as well as the spreading apart of the suction pods may occur concurrently or almost concurrently through the tensioning of a single cable. Additional embodiments of the method, system and its components are shown.

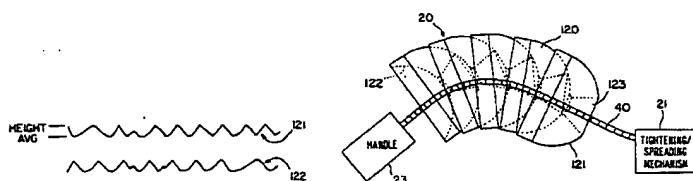

WO 00/15119 A3



KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW.

(88) Date of publication of the international search report:
31 May 2001

(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

(15) Information about Correction:

Previous Correction:

see PCT Gazette No. 34/2000 of 24 August 2000, Section II

Published:

— With international search report.

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 99/20305

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61B17/02

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 0 791 330 A (CARDIOTHORACIC) 27 August 1997 (1997-08-27)	1-16, 78, 79, 82-88, 110-120, 152-156, 158-162, 173-175, 178, 182-186
Y		63-67, 94, 96, 148, 149, 176, 177
A	column 37; figures 10B, 30, 42, 65	
A	figures 33, 75	24, 163
	figure 32C	36, 123, 164
X	figure 32B	34, 57, 58, 121,
	-/--	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

26 April 2000

Date of mailing of the international search report

11. 05. 2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Barton, S

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 99/20305

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	figure 32C	147 35, 59, 122
X	abstract; figure 60	89, 90
A	column 14, line 28	93, 99
A	figures 1B, 44	98
X	figures 32, 1B	104-106, 157
X	column 31, paragraph 2; figure 32	
X	DE 297 08 050 U (RIESS) 17 July 1997 (1997-07-17)	187, 191, 192
Y		94, 96, 176, 177
A	figures 3, 4, 10	34-36, 123, 164, 193
Y	US 5 727 569 A (BENETTI) 17 March 1998 (1998-03-17) cited in the application figures 8, 9	63-67, 148, 149
A	figure 7A	80, 150
A	WO 98 10705 A (MINNESOTA SCIENTIFIC) 19 March 1998 (1998-03-19) abstract; figures 1, 2, 4	24, 163, 190
A	WO 98 17182 A (GENZYME) 30 April 1998 (1998-04-30) page 15, last paragraph; figure 16	24
A	EP 0 808 606 A (USSC) 26 November 1997 (1997-11-26) figures 41, 42, 50	90, 93, 99
A	EP 0 167 345 A (MICRA) 8 January 1986 (1986-01-08) page 7	92, 93, 99, 100
A	US 3 786 815 A (ERICSON) 22 January 1974 (1974-01-22) column 1, line 44 -column 2, line 15	91
A	US 4 711 247 A (FISHMAN) 8 December 1987 (1987-12-08) column 3, paragraph 2	107
A	US 3 951 138 A (APOKOV) 20 April 1976 (1976-04-20) abstract; figure 1	104, 105, 155, 157
A	US 5 749 892 A (VIERRA) 12 May 1998 (1998-05-12)	
	--- -/--	

INTERNATIONAL SEARCH REPORT

In. .tional Application No

PCT/US 99/20305

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 98 27869 A (UNIVERSITY OF MASSACHUSETTS) 2 July 1998 (1998-07-02) ---	
A	WO 97 10753 A (MEDTRONIC) 27 March 1997 (1997-03-27) cited in the application ---	
P,X	WO 99 16367 A (ALLIANCE) 8 April 1999 (1999-04-08) page 5, line 6 - line 9; figures 1,7,12,13 ---	1,94-97, 155,176, 177, 187-189, 191
P,X	EP 0 920 835 A (ETHICON) 9 June 1999 (1999-06-09) paragraphs '0036!', '0040!; figures 12,13 -----	1,63,148

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 99/20305

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☒ Claims Nos.: 127-135
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
Numbers 127-135 omitted from claims numbering sequence
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☒ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☒ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. Claims: 1-16,78,79,82-88,110-120,152-154,155,156,158-162,
173-175,178,182-186

Tissue immobilising system with movable paddles, in particular with a combination of malleable conforming and suction gripping

2. Claims: 1,12,17-23

Tissue immobilising system with movable paddles, with spreading means including a spreadable saddle

3. Claims: 1,24-33,155,163

Tissue immobilising system with movable paddles, with independent spreading of first and second paddles

4. Claims: 1,36-52,110,123-142,164-172

Tissue immobilising system with movable paddles, with hinged spreading means

5. Claims: 1,53-56,81,87,110,111,143-146,151

Tissue immobilising system with movable paddles, with simultaneous paddle spreading and arm locking

6. Claims: 1,34,57,58,110,121,147

Tissue immobilising system with movable paddles, with parallel paddle spreading

7. Claims: 1,35,59-62,110,122

Tissue immobilising system with movable paddles, with non-parallel paddle spreading

8. Claims: 1,63-77,110,148,149

Tissue immobilising system with movable paddles, with multiple suction ports on a single surface

9. Claims: 1,80,110,150

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

Tissue immobilising system with movable paddles, with special arrangement of suction source, suction port and paddle and port surfaces

10. Claims: 1,89-93,99-103

Tissue immobilising system with movable paddles, with special construction of flexible arm

11. Claims: 1,94-98,155,176,177,178-181,187-194

Tissue immobilising system with movable paddles, with spreading actuator remote from paddles

12. Claims: 1,104-109,155,157

Tissue immobilising system with movable paddles, with paddle with puncturing and dispensing capability

INTERNATIONAL SEARCH REPORT

Information on patent family members

Int. Application No

PCT/US 99/20305

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 791330	A	27-08-1997	US 5894843 A	20-04-1999
			AU 1480597 A	28-08-1997
			BR 9701028 A	03-11-1998
			CA 2197614 A	21-08-1997
			JP 10005230 A	13-01-1998
			NO 970753 A	21-08-1997
			US 6036641 A	14-03-2000
DE 29708050	U	17-07-1997	WO 9849947 A	12-11-1998
			EP 0981297 A	01-03-2000
US 5727569	A	17-03-1998	AU 1478797 A	28-08-1997
			BR 9701030 A	03-11-1998
			CA 2197608 A	21-08-1997
			EP 0791329 A	27-08-1997
			JP 11019096 A	26-01-1999
			NO 970751 A	21-08-1997
			US 5906607 A	25-05-1999
			US 6032672 A	07-03-2000
WO 9810705	A	19-03-1998	US 5899627 A	04-05-1999
			EP 0866673 A	30-09-1998
			JP 2000501323 T	08-02-2000
WO 9817182	A	30-04-1998	AU 4599697 A	15-05-1998
			EP 0944356 A	29-09-1999
EP 808606	A	26-11-1997	US 5967973 A	19-10-1999
			AU 1911497 A	30-10-1997
			CA 2202833 A	26-10-1997
			JP 10052430 A	24-02-1998
			AU 1911597 A	30-10-1997
			CA 2202838 A	26-10-1997
			EP 0803228 A	29-10-1997
			JP 10033543 A	10-02-1998
			US 5947896 A	07-09-1999
EP 167345	A	08-01-1986	GB 2166190 A	30-04-1986
			JP 61092306 A	10-05-1986
US 3786815	A	22-01-1974	NONE	
US 4711247	A	08-12-1987	AU 615161 B	26-09-1991
			AU 7356987 A	09-11-1987
			BR 8707670 A	15-08-1989
			CA 1306673 A	25-08-1992
			DK 663887 A	16-12-1987
			EP 0303618 A	22-02-1989
			FI 884802 A	18-10-1988
			JP 1502718 T	21-09-1989
			WO 8706115 A	22-10-1987
			US 5605160 A	25-02-1997
			US 5588441 A	31-12-1996
			US 5027826 A	02-07-1991
			US 5154181 A	13-10-1992
			US 5735288 A	07-04-1998
			US 5335670 A	09-08-1994

INTERNATIONAL SEARCH REPORT

Information on patent family members

Int. .onal Application No

PCT/US 99/20305

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 3951138 A	20-04-1976	SU 449525 A	15-05-1976
		CA 1034825 A	18-07-1978
		CH 583545 A	14-01-1977
		DE 2434883 A	27-03-1975
		FR 2238463 A	21-02-1975
		GB 1457365 A	01-12-1976
		IT 1034067 B	10-09-1979
US 5749892 A	12-05-1998	US 6017304 A	25-01-2000
		US 5807243 A	15-09-1998
WO 9827869 A	02-07-1998	AU 5803798 A	17-07-1998
WO 9710753 A	27-03-1997	US 5836311 A	17-11-1998
		AU 7241496 A	09-04-1997
		BR 9610670 A	06-07-1999
		CA 2232580 A	27-03-1997
		CN 1198664 A	11-11-1998
		EP 0939605 A	08-09-1999
		JP 11511366 T	05-10-1999
		NO 981289 A	19-05-1998
		US 6015378 A	18-01-2000
		US 5927284 A	27-07-1999
WO 9916367 A	08-04-1999	AU 9664398 A	23-04-1999
EP 920835 A	09-06-1999	US 6007486 A	28-12-1999
		AU 8831798 A	29-04-1999
		CA 2249655 A	07-04-1999
		JP 11192226 A	21-07-1999



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 7 : A61B 17/02	A2	(11) International Publication Number: WO 00/15119
		(43) International Publication Date: 23 March 2000 (23.03.00)

(21) International Application Number: **PCT/US99/20305**

(22) International Filing Date: **3 September 1999 (03.09.99)**

(30) Priority Data:
60/100,443 **15 September 1998 (15.09.98)** **US**

(63) Related by Continuation (CON) or Continuation-in-Part (CIP) to Earlier Application
US **60/100,442 (CIP)**
Filed on **15 September 1998 (15.09.98)**

(71) Applicant (for all designated States except US): **MEDTRONIC, INC. [US/US]; 7000 Central Avenue NE, Minneapolis, MN 55432 (US).**

(72) Inventors; and

(75) Inventors/Applicants (for US only): **BORST, Cornelius [NL/NL]; Obrechtlaan 55, NL-3723 KB Bilthoven (NL). MANSVELT-BECK, Hendricus, J. [NL/NL]; Bildzigt 14, NL-3721 KK Bilthoven (NL). BOONE, Eric [US/US]; 7258 Walnut Avenue, Jenison, MI 49428 (US). GOODMAN, Jack [US/US]; 3228 Cottontail Court, Ann Arbor, MI 48103 (US). HALL, John, D. [US/US]; 2957 Longstreet Avenue SW, Wyoming, MI 49509 (US). O'NEILL,**

William, G. [US/US]; 7267 Cuesta Way Drive, Rockford, MI 49341 (US). TESTA, Vincent, J. [US/US]; 510 North Center Drive, Grand Rapids, MI 49544 (US). VROEGOP, Eric [US/US]; 105 Birchwood, Holland, MI 49423 (US).

(74) Agents: **JARO, Michael, J. et al.; Medtronic, Inc. MS301, 7000 Central Avenue N.E., Minneapolis, MN 55432 (US).**

(81) Designated States: **AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).**


Published

Without international search report and to be republished upon receipt of that report.

(54) Title: **METHOD AND APPARATUS FOR TEMPORARILY IMMOBILIZING A LOCAL AREA OF TISSUE**

(57) Abstract

The invention is a method and apparatus for performing beating heart surgery, in which a single articulating arm supports multiple suction pods. Once the suction pods are applied to the heart surface, tightening a cable fixes the arm in place. Then, the suction pods may be spread apart from each other to tighten the surface of the cardiac tissue lying between the suction pods. In one embodiment, fixation of the arm as well as the spreading apart of the suction pods may occur concurrently or almost concurrently through the tensioning of a single cable. Additional embodiments of the method, system and its components are shown.

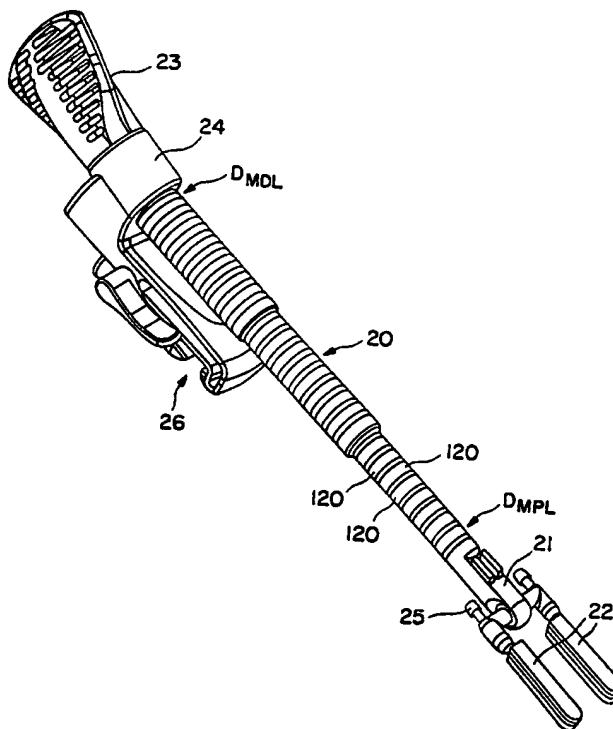

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

METHOD AND APPARATUS FOR TEMPORARILY
IMMOBILIZING A LOCAL AREA OF TISSUE

FIELD OF THE INVENTION

5 The present invention generally relates to surgery on body tissues and organs. More specifically, the present invention relates to a method and apparatus for temporarily immobilizing a local area of tissue subject to motion, such as the heart wall, which permits a surgical procedure to be performed on that local area of tissue.

10 **BACKGROUND OF THE INVENTION**

Coronary artery disease remains the leading cause of morbidity and mortality in Western societies. Coronary artery disease is manifested in a number of ways. For example, disease of the coronary arteries can lead to insufficient blood flow to various areas of the heart. This can lead to the discomfort of angina and the risk of ischemia.
15 In severe cases, acute blockage of coronary blood flow can result in irreversible damage to the myocardial tissue including myocardial infarction and the risk of death.

A number of approaches have been developed for treating coronary artery disease. In less severe cases, it is often sufficient to merely treat the symptoms, with pharmaceuticals, or treat the underlying causes of the disease, with lifestyle
20 modification. In more severe cases, the coronary blockage can be treated endovascularly or percutaneously using techniques such as balloon angioplasty, atherectomy, laser ablation, stents, and the like.

In cases where these approaches have failed or are likely to fail, it is often necessary to perform a coronary artery bypass graft procedure. This procedure
25 generally consists of the following steps: First, direct access to the heart is achieved. This is usually done by opening the chest by median sternotomy and spreading the left and right rib cage apart; and opening the pericardial sac to achieve direct access to the heart.

Next, a blood vessel or vessels for use in the graft procedure are mobilized
30 from the patient. This usually entails mobilizing either a mammary artery or a saphenous vein, although other graft vessels may also be used.

Next, a heart-lung or cardiopulmonary bypass is performed. This usually entails arterial and venous cannulation, connecting the bloodstream to a heart-lung machine, cooling the body to about 32 degrees Celsius, cross-clamping of the aorta and cardioplegic perfusion of the coronary arteries to arrest and cool the heart to about 4 degrees Celsius. The arrest or stoppage of the heart is generally required because the constant pumping motion of the beating heart would make surgery upon the heart difficult in some locations and extremely difficult if not impossible in other locations

Once cardiac arrest is achieved, then a graft (or grafts) is attached to the relevant portions of a coronary artery (or arteries) followed by weaning from the cardiopulmonary bypass, restarting the heart and decannulation. Finally the chest is closed.

One area which may create difficulties for the patient, and extra expense and time for the procedure, involves the cardiopulmonary bypass. In a cardiopulmonary bypass all the patient's blood, which normally returns to the right atrium, is diverted to a system which supplies oxygen to the blood and removes carbon dioxide and returns the blood, at sufficient pressure, into the patient's aorta for further distribution into the body. Generally such a system requires several separate components, including an oxygenator, several pumps, a reservoir, a blood temperature control system, filters as well as flow, pressure and temperature sensors.

Problems may develop during cardiopulmonary bypass due to the reaction blood has to non-endothelially lined surfaces, i.e. surfaces unlike those of a blood vessel. In particular, exposure of blood to foreign surfaces results in the activation of virtually all the humoral and cellular components of the inflammatory response, as well as some of the slower reacting specific immune responses. Other complications from cardiopulmonary bypass include loss of red blood cells and platelets due to shear stress damage. In addition, cardiopulmonary bypass requires the use of an anticoagulant, such as heparin. This may, in turn, increase the risk of hemorrhage. Finally cardiopulmonary bypass sometimes necessitates giving additional blood to the patient. The additional blood, if from a source other than the patient, may expose the patient to blood born diseases.

Due to the risks incurred during cardiopulmonary bypass, others have attempted to perform a coronary artery bypass graft procedure without cardiac arrest and cardiopulmonary bypass. For example, Trapp and Bisarya in "Placement of Coronary Artery Bypass Graft Without Pump Oxygenator", *Annals Thorac. Surg.* Vol. 19, No. 1, (Jan. 1975) pgs. 1-9, immobilized the area of the bypass graft by encircling sutures deep enough to incorporate enough muscle to suspend an area of the heart and prevent damage to the coronary artery. More recently Fanning et al. in "Reoperative Coronary Artery Bypass Grafting Without Cardiopulmonary Bypass", *Annals Thorac. Surg.* Vol. 55, (Feb. 1993) pgs. 486-489 also reported immobilizing the area of the bypass graft with stabilization sutures.

Current beating heart bypass surgery techniques demand relatively motionless epicardial tissue in the immediate vicinity of an anastomosis. Several systems are presently available which attempt to immobilize epicardial tissue in the immediate vicinity of an anastomosis through a simple mechanical fork. One of the many such systems presently available includes the Access™ system available from CardioThoracic Systems Inc., Cupertino, California. Such a system stabilizes the heart by pressing a fork downwards onto the heart surface. Through this pressure the region of the epicardium between the fork is immobilized. Commercially available systems use short arms mounted to retractors in close proximity to the chest cavity. Mechanical fork systems only operate successfully on vessels that can be immobilized by applying pressure in a downward direction. These systems are very useful for operations on the anterior portion of the heart (such as the left anterior descending artery). However, fork systems are limited in their ability to maneuver a vessel into better view or for operating on the posterior portion of the heart. That is, fork systems are limited in their ability to "present" a vessel to the surgeon. This is a even greater drawback since fork systems stabilize only through compression, therefore often pushing downwards the are of surgical interest. In addition, compression of the heart can lead to diminished cardiac output, presenting a further risk to the patient's well-being. Finally, such systems, to date, have often featured rigid, inflexible arms which often interfere with the view or movements or both of the surgeon.

Suction stabilization systems, such as the Medtronic Octopus® Tissue Stabilizer and Accessories (available from Medtronic, Inc., Minneapolis, Minnesota USA), use comparatively long, dual reusable articulating arms configured with clamps at their distal ends to secure suction based tissue stabilizers. During use, the arms are typically secured to a rail on the side of the operating table. The suction grips and immobilizes the surface of the heart. Additionally, the system allows the surgeon to manipulate the anastomosis site into better view by rotating and supporting the heart. The system also allows the surgeon to apply tension to the tissue between the stabilizers. Thus, the system is much more versatile than mechanical fork style systems. The suction paddles or pods can attach to and immobilize the heart, and can be used to manipulate the heart into better position so that the more difficult to reach vessels can be bypassed.

Many surgeons have used the Medtronic Octopus® Tissue Stabilizer system to perform as many as five or six vessel bypasses. Some surgeons, in fact, report using the product on 50-90% of their cases. Nonetheless such a system is still in need of improvement. For example, such a system was relatively more cumbersome to set up than desired, requiring each stabilization arm to be individually fixed or immobilized. Moreover, because each arm worked individually, spreading the arms relatively apart was more difficult than desired. Finally, because the degree of spreading was not limited in any way, surgeons could spread the paddles apart at greater distance than desired, causing one or both paddles to spontaneously lose capture of the tissue.

While these past products and attempts have achieved some success, their still exists a need to provide a method and apparatus for performing beating heart surgery which readily and quickly permits the immobilization or stabilization of a local area of tissue.

The present invention concerns an advanced system for immobilizing or stabilizing a local area of tissue.

SUMMARY OF THE INVENTION

The invention is a method and apparatus for performing beating heart surgery, in which a single articulating arm supports multiple suction paddles or pods. Once the

suction pods are applied to the heart surface, tightening a cable fixes the arm in place. Then, the suction pods may be spread apart from each other to tighten the surface of the cardiac tissue lying between the suction pods. In one embodiment, fixation of the arm as well as the spreading apart of the suction pods may occur concurrently or almost concurrently through the tensioning of a single cable. Additional embodiments of the method, system and its components are shown.

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other aspects of the present invention will best be appreciated with reference to the detailed description of the invention in conjunction with the accompanying drawings, wherein:

FIGS. 1A through 1E show various views of a preferred embodiment of the invention.

FIG. 2 is an alternate embodiment of the present invention.

FIG. 3 is an exploded perspective view of the cable tensioning and device clamping mechanisms.

FIG. 4 is a perspective view of the first of three preferred embodiments for tightening/spreading mechanism.

FIG. 5 is an exploded perspective view of the tightening components of **FIG. 4**.

FIG. 6 is a perspective view of the second of three preferred embodiments for tightening/spreading mechanism.

FIG. 7 is an exploded perspective view of the tightening components of **FIG. 6**.

FIG. 8 is a perspective view of the third of three preferred embodiments for tightening/spreading mechanism.

FIG. 9 is an exploded perspective view of the tightening components of **FIG. 8**.

FIGS. 10-45 show additional features and alternative embodiments of the present invention.

The **FIGS.** are not necessarily to scale.

DETAILED DESCRIPTION OF THE PRESENT INVENTION

The present invention is a method and apparatus for performing beating heart surgery, in which a single articulating arm supports multiple suction pods. Once the suction pods are applied to the heart surface, tightening a cable fixes the arm in place. Then, the suction pods may be spread apart from each other to tighten the surface of the cardiac tissue lying between the suction pods. In one embodiment, fixation of the arm as well as the spreading apart of the suction pods may occur concurrently or almost concurrently the tensioning of a single cable. Additional embodiments of the system and its components are shown. Support for conventional aspects of the invention may be found in the enclosed documents, all of which are incorporated by reference in their entirety.

US 5,727,569 (Benetti *et al.*)

WO 95/01757 (Borst)

US 5,782,746 (Wright)

WO 97/10753 (Borst *et al.*)

Preferred embodiments of the invention are shown in the enclosed FIGS., and are described in detail below.

FIG. 1A is a perspective view of a preferred embodiment of the invention. An articulating arm 20 is attached to support 24 on the proximal end of the arm, and terminates with tightening/spreading mechanism 21 at the distal end of the arm. On the opposite, more proximal, end of support 24 is handle 23. Distally beyond tightening/spreading mechanism 21 is a plurality (as shown, two) of suction paddles or pods 22. Each suction pod 22 can be connected to vacuum by a conventional connection 25 that lies at the proximal end of pod 22. Each pod and its suction ports may be constructed in any acceptable manner, such as the same as that used in the Medtronic Octopus™ tissue stabilizer. Clamp 26 lies below support 24 and is designed to attach the entire device to conventional surgical retractors and other similar equipment (not shown). The preferred embodiment shown in **FIG. 1A** is illustrative but not intended to be limiting insofar as the scope of the invention is concerned. For example, the handle 23 is shown in a preferred and highly stylized embodiment, but any device which performs the functions of the handle as described below would suffice.

Articulating arm 20 comprises a plurality of "ball and socket" links. FIG. 1B is a cross sectional view of a link used in the arm of the present invention. As seen, each link 120 has a hole 123 that passes through its center. Each link 120 comprises, on its distal end, a hemispherical protrusion 121; and on its proximal end, a hemispherical indentation 122. The hemispherical shapes of adjacent links are nearly identical, such that the links rotate smoothly against one another provided they are not under undue tension with each other.

Turning now to FIG. 1C which is a partial view of a section of the links and cable showing the engagement of the cable with the side wall of the links as the arm is bent. A cable 40 passes through hole of all of the links and is connected between the handle 23 and the tightening/spreading mechanism 21. Rotation of handle 23 tightens the cable and causes the links to hold against each other in place. Immobilization of the links relative to each other during tightening of the cable is facilitated by the shape of the hole 123. As seen, hole is flared, having a larger opening with the surface of the hemispherical protrusion 121 and a smaller opening through the surface of the hemispherical indentation 122. The links, as seen in FIG. 1A, vary in size along the length of the arm, with the links in the most proximal portion of the arm being largest, the links in the most proximal portion the smallest and the middle portion somewhere in between. In the preferred embodiment the links have the following outer diameters and radius of curvature for the hemispherical protrusion and radius of curvature for the hemispherical indentation along each of these portions as follows:

Portion of arm	R ₁ (inches)	R ₂ (inches)	DIA(inches)
Most distal portion	0.251	0.250	0.514
Middle portion	0.313	0.311	0.637
Most proximal portion	0.317	0.374	0.763

In the preferred embodiment, the links are fabricated out of highly rigid engineered

thermoplastics such as glass filled Ultem™ (available from GE Plastics, Pittsfield, Massachusetts.) Preferably the highly rigid engineered thermoplastics includes at least 20% glass fiber, and better still at least 30% glass fiber. This material offers stiffness comparable to metal systems, and yet can be manufactured at costs that allow for single use disposability. The cable is preferably a multi-stranded stainless steel cable having between approximately 7 to 19 strands. The links and cable may also be manufactured from other materials, including any other suitable highly engineered polymers including any number of available liquid crystal polymers for the links, as well as many other types of cables, including bundle stranded, braided or cabled titanium as well as Kevlar™ for the cable.

The preferred embodiment also employs a textured surface molded or otherwise formed into the hemispherical features of the links. When the links are pulled together during tightening, the texturing causes an increase in coefficient of friction between the adjacent spherical surfaces. This has the highly desirable benefit of increasing overall system stiffness. This is depicted in FIG. 1D, which depicts the roughened surfaces between the ball and socket, such that in tension, the elements are more securely linked together. As seen, in the preferred embodiment, the texture provided is irregular, that is, the texture is non-uniform, and has an average height spanning approximately (peak to valley) of between 20 to 100 microns, with an average height ($height_{avg}$) spanning approximately 40 microns preferred. As seen in FIG. 1E, moreover, in an alternative embodiment texture may be provided through a symmetrical structure, depicted here as a series of interlocking dimples 127 and hemispheres 128. Other geometries may also be used, including both surface having the same elements, such as hemispheres, as well as other shapes, including notches or grooves, to name only a few.

In this embodiment, articulating arm links 120 have a decreasing outer diameter from the proximal portion to distal end portion of the arm. This is also seen in FIG. 1A, where outer diameter of the most proximal link portion D_{MPL} is larger is that the outer diameter of the middle link portion D_{MLP} which, in turn, is larger is that the outer diameter of the most distal link portion D_{MDL} . Decreasing the link diameter allows a lower profile assembly that improves the ability of the surgeon to use the

device without unduly restricting accessibility to the surgical site while further ensuring adequate rigidity. In the preferred embodiment D_{MPL} is approximately 0.75 inches, D_{MDL} is approximately 0.50 inches and the D_{MLP} a outer diameter of approximately 0.625 inches, and the total arm length is approximately 10.25 inches with the pods and approximately 9 inches without the pods. Further, in the preferred embodiment most proximal link portion features 19 links, middle link portion features 4 links, and most distal link portion features 3 links.

In an alternate embodiment, as shown in FIG. 2, the links of articulating arm 20 are covered with a thin walled elastomeric sheath 27. The sheath serves to prevent fragile sutures from catching on the edges where the links join. Sheath is preferably manufactured of silicone rubber, although other materials, such as latex rubber or polyurethane or even collagen, may also be used.

FIG. 3 is an exploded perspective view of the cable tensioning and device clamping mechanisms. Tension is applied to cable 40 by a torque screw and nut configuration at the proximal end of the device. Cable 40 passes through mount 24, and then through the bore of torque screw 25, and terminates in a swaged connector 27. In the preferred embodiment shown, the torque screw interacts with a corresponding nut portion 13 which is integrally formed within handle 23, although an embodiment in which handle 23 turned a separate nut is within the scope of the invention. Torques screw preferably is threaded at 12 threads per inch. As handle 23 is rotated, torque screw 25 engages nut portion 13 and advances proximally into handle 23, tensioning cable 40. It is preferred, for safety purposes, for the degree or amount of cable tensioning in the system to be limited. In the preferred embodiment this is accomplished by sizing housing 24, torque screw 25, and handle 23 such that torque screw 25 may advance into handle 23 along nut portion only a predetermined amount. In such a manner the system is configured so that the cable may not be over-tensioned, i.e., tightening of cable 40 is limited so as to remain comfortably below the rated strength of cable 40.

The torque screw, through the mechanical advantage of a 12 thread per inch torque screw allows cable tensions as high as 500 lb. to be applied by hand. While

the actuation is somewhat slower than possible other type actuators (e.g. scissors-type actuator) the high tension in the cable optimizes arm rigidity.

Arm rigidity is further enhanced through the interplay between the multi-stranded cable riding on the inner diameter of the plastic segments. The multi-stranded cable riding on the inner diameter of the plastic segments induces additional friction which optimizes stability. As the cable is tensioned at high load values (>200 lb.), the cable digs into the inner diameter of the softer plastic of the segments. This is depicted above in regards to FIG. 1C which is a partial view of a section of the links and cable showing the engagement of the cable with the side wall of the links as the arm is bent. Since the cable is striated with typically 7-19 strands, the result is a strong interlocking of cable and plastic segments. The interlocking of the stranded cable to the plastic segment increases the coefficient of friction between cable and plastic segment. This further locks up segments to each other since they cannot slide easily along the cable. Thus enhancing arm rigidity. Below sufficient cable tension, however, the cable does not dig into the links and cause the strong increase in coefficient of friction. Additional embodiments of the invention may also feature cables of greater surface roughness, as well as sheathing the cable in materials sheaths having a greater coefficient of friction than the cable itself. Such friction enhance sheaths are particularly believed useful where cables other than stranded cables are used, such as Kevlar™ cables, as mentioned above.

The complete device is designed to be clamped to a wide variety of commonly used sternal retractors. Clamping mechanism 26 comprises mating portions of mount 24 and a movable jaw 28, each configured to provide half of a dovetail shaped groove. Movable jaw 28 is attached to mount 24 by a center pin 29 that passes through a groove 28 in the movable jaw 28. Center pin 29 also passes through conical spring washer 30. Groove 35 allows movable jaw 28 slide back and forth, permitting mounting to retractor elements of varying width. Center pin 29 comprises a cross hole 31. Cam pin 36, which is rigidly affixed to a knob 33, passes through cross hole 31, capturing together the movable jaw 28 and the mount 24. Cam pin 36 has an off-axis lobe 32 which induces upward movement on center pin 29 when knob 33 is advanced forward (in the FIG. 3, clockwise) to a horizontal position parallel to the cable 40.

This upward motion compresses spring washer 30, which pulls the two halves of the clamp together. This induces, onto the retractor, both horizontal and vertical clamping forces in the dovetail features of the clamp halves, securing the clamp in place.

Movable jaw 28 is additionally provided with dual compression springs 34 which bias the clamp to a fully forward position. This provides more convenient mounting of the clamp, and also ensures a more reliable connection between the mount and retractor element.

FIG. 4 is a perspective view of the first of three preferred embodiments for tightening/spreading mechanism 21. **FIG. 5** is an exploded perspective view of the tightening components of **FIG. 4**. The embodiment of **FIGS. 4 and 5** provides simultaneous parallel translation of suction pods 22, along the x-axis, by rotation of wheel 5. This spreading/closing action can be performed when the articulating arm 20 is either loose or tight. Additionally, when articulating arm 20 is loose, suction pods 22 can be independently rotated about the yz plane. This allows the surgeon wide flexibility in the manner of approach to the anastomosis site. Because the spreading action is parallel, the cardiac tissue tensioning effect is uniform across the anastomosis site (below and between suction pods 22).

Cable 40 terminates at tabbed element 4 by cable ball 50. Tensioning of cable 40 causes tabbed element 4 to move proximally. Ears 51 of tab element 4 mate into slot 52 of sling 10. Thus, tensioning or pulling on cable imparts tension or pulling back on sling 10. Sling 10 wraps around two pod guides 6, capturing guides 6 against head link 3. As cable 40 is tightened, sling 10 pulls pod guides 6 ever more firmly into head link 3 until they can no longer rotate. In the preferred embodiment, pod guides 6 are configured with square holes. These square holes are provided to mate with square projections on the pod guides and thus guide the movement of suction pods 22 in and out. The square shape serves to prevent rotation of suction pods 22 in the yz plane once cable 40 has been tightened. Additionally, to prevent minor oscillations of suction pods 22 in the yz plane due to small clearances between pod guides 6 and suction pods 22, pod guides 6 each include small torsion springs 10 which bias suction pods 22 to one side of the respective pod guide 6. Suction pods 22

have a square element, which projects into the center of the spreader mechanism through pod guides 6.

Wheel 5 is located between the two pod guides 6. Wheel 5 has a threaded rod projecting through its center along the x-axis. To one side of wheel 5, the threaded rod has a right hand thread, and to the other side, a left hand thread. These threads mate with respectively threaded holes in the projections of the two suction pods 22. Rotating wheel 5 causes the pods to move simultaneously apart or together in parallel. Vacuum connections to suction pods 22 are made via barbed connections 25 at the proximal end of suction pods 22.

FIG. 6 is a perspective view of the second of three preferred embodiments for tightening/spreading mechanism 21. **FIG. 7** is an exploded perspective view of the tightening components of **FIG. 6**. The embodiment of **FIGS. 6** and **7** provides sequential tightening of the articulating arm concurrently or closely followed by angular separation of suction pods 22 in the xy plane, by tightening of handle 23. When articulating arm 20 is loose, suction pods 22 are free to rotate in the yz plane, and to a lesser extent in the xz and xy planes. This allows the surgeon even greater flexibility on approaching the anastomosis site. The tightening of cable 40 causes the spreading action. Because the spreading action is rotational, the tensioning effect will be uneven, being generally V-shaped, that is more pronounced at the distal end of the anastomosis site.

Cable 40 terminates in tabbed element 13. Tensioning of the cable causes the tabbed element to move proximally, pulling back on sling 14. The sling wraps around the split ball 225 of pods, capturing the split ball. In its relaxed state, when the stainless cable is loose, relatively little friction exist between split ball 225, inner cavity of sling 14 and outer spherical surface of head link 12 so that split ball 225 is relatively able to be moved or rotated therein. In the preferred embodiment, the outside diameter of split ball is equal to the diameter of the spherical cavity defined within sling and head link, preferably these diameters are all approximately 0.193 inches. As the cable is tightened, however, the sling cinches down over the split ball compressing the split ball into the sling and head link 12. As the split ball 225 is compressed, the split 226 closes, causing suction pods 22 to splay angularly outward.

In the preferred embodiment split ball 225 is made from non-glassed filled Ultem™ (available from GE Plastics, Pittsfield, Massachusetts.)

In a preferred embodiment, a compressible (preferably elastomeric) disk 15, is mounted between sling 14 and head link 12. The preferred material for disk 15 is
5 silicone with a durometer of 80, although other materials or durometers or both may also be selected. Disk 15 preferably sits or mates into a compression limiter 41, depicted here as a stainless steel cup 41, which functions to limit the total amount to which the disk may be compressed. That is, disk 15 is sized to fit within cup so as to be able to be compressed an amount no greater than the depth of the cup. In the
10 preferred embodiment, allowed to be compressed approximately no more than 0.040 inches. Of course, other sizes and material may also be selected. The identity, size, and other materials properties of the elastomeric disk 15 and cup (if used, for example, cup could be integrated into head link or cable tab) are chosen such that disk 15 it is crushed between head link 12 and sling 14 before the split ball is compressed.
15 This causes articulating arm 20 to become firm before the spreading or other moving of the suction pods 22 begins, adding a desired degree of control to the system. Vacuum connections to suction pods 22 are made via barbed connections 25 at the proximal end of suction pods 22.

FIG. 8 is a perspective view of the third of three preferred embodiments for
20 tightening/spreading mechanism 21. **FIG. 9** is an exploded perspective view of the tightening components of **FIG. 8**. The embodiment of **FIGS. 8** and **9** provides independent rotational spreading of the suction pods (not shown in these two **FIGS.**) in any plane about a point of rotation at the center of the mechanism. When articulating arm 20 is loose, the suction pods 22 will move freely. Because the suction
25 pods 22 are not linked together in this embodiment, they are able to conform to surfaces of the heart where the suction pods would not be co-planar. This provides more secure mounting of the suction pods on areas of the heart with small radii of surface curvature.

Cable 40 terminates at tabbed element 17. Tensioning of the cable causes
30 tabbed element 17 to move proximally, pulling back on sling 18 through the interaction of ears 51 and groove 52. Pod mounts 19 each contain hemispherical

sockets that fit smoothly about ball 50 and are captured between sling 18 and head link 16. Tensioning of cable 40 causes tabbed element 17 to move proximally, pulling back on sling 18, pinching ball 50 and the pod elements firmly together. In use, the surgeon would partially tighten the cable, and then pinch together the pod finger tabs 27 to achieve the desired amount of spreading. In a preferred embodiment, a compressible disk is used as described previously. Vacuum connections to the suction pods are made via barbed connections 25.

FIG. 10 depicts the relationship between rigidity of the articulating arm and the spreading apart of the suction pods 22 shown above in **FIG. 1A**. As seen the present invention is designed so to provide a particular relationship between the rigidity of articulating arm and the spreading of suction pods. In the embodiment shown in **FIGS 6 & 7** the initial relationship between rigidity and spread is linear until a spreading point, seen here as Q, is reached. Thereafter a non-linear relationship is seen. In this embodiment there is thus a simultaneous change in the rigidity of the arm and the spreading of the pods.

FIGS. 11 & 12 depict the relationship of rigidity and spreadability in a further embodiment of the present invention. As seen in this embodiment the articulating arm undergoes a transformation of rigidity from loose flexibility to firm flexibility at time B₁. Thereafter, at time B₂ articulating arm undergoes a transformation of rigidity from firm to hard. Continuing tightening of the handle (which controls rigidity and spread in the embodiment shown in **FIGS. 1-7**) does not cause the arm to become appreciatively more rigid. In contrast, the spreadability of the suction pods is depicted in **FIG. 12** and is seen, in particular, to occur at a lag from the transformation of rigidity. In particular, as seen at B₁ the rigidity is increased from loose to firm while the spread of the suction pods does not occur until time C₁ that is, turning of handle 23 to reduce the flexibility of the part of the articulating arm from loose to firm does not cause an appreciable spread until a time thereafter, here seen as C₁. The particular relation between rigidity and spread may be selected to occur in any favorable matter. Practically speaking, the relationship between rigidity and spread may be a matter of choice which is best left to the surgeon. Thus, the present invention permits this relationship to be tailored as desired though the selection of

among the following factors: in the present invention shown in FIG. 1A and thereafter shown in particular regard in FIGS. 6 & 7, the relationship of rigidity and spread may be controlled through the particular design and selection of the arm links and texture, split ball and hinge, split ball and split or gap, washer and cup as well as any of their materials.

This is seen in FIGS. 13 through 21, which show the split ball 225 of the preferred embodiment (FIG. 13 through 16) and alternative designs. As seen FIG. 13 is a detailed perspective of split ball 225 shown assembled in a stabilization system. FIG. 14 is a plan view of the split ball 225 shown in FIG. 13 from an overhead position. This view shows the split or gap 226 within split ball and the hinge 227. The size of hinge 227 and split or gap 226 define the actuation of the pods mounted to the split ball and further the degree of force required. These elements, along with other elements of the present invention, may be tailored to provide the particular actuation and performance characteristics deemed suitable for a surgeon or surgeons. FIG. 15 is a cross sectional view of split ball 225 shown in FIG. 13 along line 15-15. In the preferred embodiment gap 226 has a minimum thickness T_{226} of between 0.010 – 0.100 inches, with 0.040 inches preferred, while hinge 227 has a thickness T_{227} of between 0.220 – 0.010 inches, with 0.110 inches preferred. FIG. 16 is a two-dimensional plot of the gap along the outer surface of the split ball. As seen, in this embodiment, gap is symmetrical along the outer surface.

Many other alternative embodiments of the split ball may be provided. FIG. 17 shows one embodiment in which the hinge is positioned above the center line of the split ball. FIG. 18 shows one embodiment in which the hinge is positioned below the center line of the split ball. FIG. 19 shows one embodiment in which the hinge is positioned at the backside of the split ball, as compared to the embodiment seen in FIG. 15. In this embodiment the tension on the cable would cause the front of the split ball to be compressed, thereby spying inwardly the suction pods. Such pod movement may be useful for squeezing tissue between the pods. Besides positioning the gap and thus the hinge at various portions within the split ball, gap may further be fashioned so as to be larger at a top end and smaller or narrower at a bottom end. FIG. 20 shows an embodiment in which gap 227 is wider at the upper end (above the

0 degree line) and narrower at the lower end (below the 0 degree line). FIG. 21 is a two-dimensional plot of the gap along the outer surface of the split ball. As seen, in this embodiment, gap is non-symmetrical along the outer surface, larger at its upper end and narrower in its bottom end.

5 FIG. 22 depicts an alternative embodiment of the present invention. In this embodiment suction pods are separated, and not joined such that each suction pod is free to be moved within the Y Z plane, similar to that already shown in FIG. 4. Movement is provided through the segmented spreadable hinge 199, which is provided through the interrelationship of sling 15 and the corresponding left suction
10 pod 22L and right suction pod 22R. Spreadable hinge 199 is provided through an inter-mating ball and socket assembly, provided on respective floating pods 22R and 22L in particular a hemispherical ball 198 is provided on right suction pod 22R and a corresponding inter-mating hemispherical socket 197. As seen socket and ball are dimensioned such that they may be mated together and the smaller diameter portion
15 of ball inserted into the hemispherical opening of hemispherical socket 197. Thereafter the mated together pieces generally form a segmented hemisphere which may be disposed within the sling 15 as already described above in regards to FIGS. 6 & 7. This embodiment has advantages over that shown above in FIGS. 6 & 7 because the individual paddles 22L & 22R may be oriented along the various axis to provide
20 secure capture of the surface of the heart.

 In a further embodiment of the present invention the segmented spreadable hinge 199 as well as spreadable hinge shown above in regards to FIGS. 6 & 7 may be provided such that the suction pods move in a non-parallel fashion. One embodiment of this non-parallel movement is shown in FIG. 23. As seen in a first, non-spread,
25 orientation paddle 22L & 22R are disposed of first distance A apart. Once the spreading has been initiated through any of the various methods described above, paddles 22L & 22R shown on the disposition of FIG. 24. As seen in this disposition the closes point the paddles have to one another is at their base or proximal positions and is at a distance A + X. The distal ends of the paddles are shown at a distance
30 A+Y apart such that an angle faded exists between the longitude and the axis of each

paddle. Embodiments which may be utilized to achieve this movement are those shown above.

FIG. 30 depicts further alternative embodiment of the present invention. In this embodiment suction pods 22L & 22R may be spread and rotated such that they move from an orientation shown in **FIG. 30**, and have a distance A apart, to the orientation shown in **FIG. 31**. As seen in **FIG. 31**, at this point paddles 22L & 22R are a minimal distance $A + X1$ apart at their proximal end and a greater distance $A + X2$ apart at their distal end. Furthermore, the pods have had a relative rotation such that the bottom surface of the pods now define an angle sigma.

FIG. 32 depicts a further alternative embodiment of the present invention. In particular, **FIG. 32** is a sectional view across pod 22L shown in **FIG. 22** along line O-O. As seen, in this embodiment, pod 22L features a suction port 33 open along the bottom surface of the suction pod. Suction port 33 further communicates with a suction aperture 31. In this embodiment the total height H of the pod is minimized because the suction aperture is located along side the suction port such that the aperture exists at the point at the suction port no greater than the alternate height of the suction port opening, that is the bottom of the suction port, depicted here as 33-b is relatively above, in this figure, suction aperture 34. H is between approximately 1 and 4 millimeters, with 2-3 preferred.

FIGS. 33-37 depict alternative embodiments of the suction pods. These alternative embodiments may be used together or in any combination of any of the above and below shown suction pods. Exact usage of these types of suction pods would be at the preference of the surgeon. In **FIG. 33** an embodiment is shown in which each of the suction ports 33-1 through 33-5 have the same diameter. In this embodiment, however, the suction apertures 34-1 through 34-4 have different opening sizes into the relative suction ports. In particular, in this embodiment suction aperture 34-2 and 34-3 are relatively much larger than the corresponding suction apertures 34-1 and 34-5. The relatively larger suction apertures are provided in that they provide a more quick capture and fixation of the relevant suction port to the tissue. In contrast, suction ports having relatively smaller suction apertures require more time to effectively capture the tissue. While shown in this **FIG.** as having relatively larger

suction apertures in the two central ports, the opposite may also be provided such that the relatively larger suction apertures are at the end suction ports. The benefit of this configuration is that ports 33-1 and 33-4 are least likely to spontaneously lose capture, while the inner ports 33-2 and 33-3 will quickly achieve capture.

5 **FIG. 34** shows an additional embodiment of the present invention. In this embodiment suction pod is non-rectangular, and in particular, shown as having a relatively, tapered, elongated orientation. Furthermore, such ports are provided which have variable diameters. In particular, in this embodiment, suction port 33-1 has relatively larger diameter, and the diameter of the subsequent suction ports 33-2 at Et
10 seq. become relatively smaller until suction port 33-5 as shown as having the smallest suction port diameter. In this embodiment the corresponding suction apertures 34-1 through 34-5 are provided having a consistent diameter and those surface area opening into the suction ports. Of course, as described above these may be varied in size.

15 **FIG. 35** shows a suction pod having an ever decreasing sized suction ports and furthermore having ever decreasing sized apertures and ports.

 While suction port has been shown above as generally circular it may also be provided in other, non circular forms. In **FIG. 36** it is shown that suction port may be provide both as elliptical as well as trapezoidal configurations. In each of the
20 embodiments suction port is provided with a single suction aperture. Of course, suction aperture may be provided more than once into the same suction port.

FIG. 37 shows a suction pod having variable diameter suction ports while consistent suction apertures. In this embodiment the central suction port are much larger than the end point suction ports.

25 **FIGS. 38-40** depict an alternative embodiment of the present invention. As seen, suction pod 22 has a series of suction ports 33 as already described above. In this embodiment suction pod is made, however, from a malleable material such that the pod itself can be shaped by the surgeon prior to disposition of the pod onto the surface of the heart. It is believed that this malleability provides the surgeon with
30 increased flexibility so as to shape the pod to be conformed into or around the surface of the particular area of the heart upon which he will operate. As seen malleable pod

may further include a spring or other form of malleable but lockable member 190. In the present invention this lockable member 190 would comprise a wound coiled spring, although other materials and devices may be used, including, but not limited to, straps, band, bands, interwoven metallic members, heat set plastics, to name some
5 of other alternative materials and devices which may be used. In a first embodiment the malleable pod is constructed of PVC (poly vinyl chloride) 73 Shore A durometer and the lockable member is constructed from a hypotube made of MP35N metal alloy. In the preferred embodiment the hypotube used to carry suction to the suction ports and thus functions as a suction aperture. Alternately, the malleable pod formation
10 permits the pod itself to be moved from its first orientation, as seen in FIG. 40 at 189 to the deformed position 188. Alternatively, pod may be manufactured from many other types of materials, including silicone rubber, polyurethane, to name only a few, while lockable member may be constructed from coiled conductors, polymeric strips, or strips or ribbons or springs made from nitinol.

15 The present invention may be especially suitable for performing a surgical operation on a patient utilizing the simultaneous spreading of the device's paddles and the stiffening of the fixation arm. That is, this embodiment may permit use of the following method of performing a surgical procedure. First, the desired area of tissue is accessed, e.g. the heart and the coronary artery of interest is accessed. Next, a
20 stabilization system is placed upon the surface of the tissue, e.g. a stabilization system as shown in FIGS. 1C, 6-9 is placed upon the surface of the tissue, and in particular suction pods 22 are placed upon the surface of the tissue. Next, suction is introduced into each pod such that the surface of the tissue is captured by the first pod and the second pod. Next, the first pod and the second pod are caused to be spread relatively
25 apart while the articulating arm 20 is concurrently caused to become stiff. In the illustrated embodiment of FIGS. 1C this may be accomplished by turning distal handle 23. As already described above, turning of distal handle causes tension to be applied to cable, causing in turn first paddle and second paddle to thereafter be spread relatively apart or otherwise moved (e.g. moved together, where the exact motion
30 depends on the hinge design and the orientation of the pods or paddles) and also causing each of the links of the arm to be compressed together. The method may also

be performed where the step of causing the articulating arm to become stiffer may be performed at either a time prior to or after the step of spreading relatively apart the first pod and the second pod. Thereafter a surgical procedure may be performed. Finally, the process is reversed and the patient is closed, as is well known in the art.

5 The particular embodiment shown in **FIGS. 4 and 5** may be especially suitable for performing a surgical operation on a patient utilizing only the spreading aspect of the device' paddles and not the stabilization through the stiffening of the fixation arm. That is, this embodiment may permit use of the following method of performing a surgical procedure. First, the desired area of tissue is accessed, e.g. the heart and the
10 coronary artery of interest is accessed. Next, a stabilization system is placed upon the surface of the tissue, e.g. a stabilization system as shown in **FIGS. 4 and 5** is placed upon the surface of the tissue, and in particular suction pods 22 is placed upon the surface of the tissue. Next, suction is introduced into each pod such that the surface of the tissue is captured by the first pod and the second pod. Next, the first pod and
15 the second pod are caused to be spread relatively apart. In the illustrated embodiment this may be accomplished by turning wheel 5 to cause first paddle and second paddle to thereafter be spread relatively apart. Thereafter a surgical procedure may be performed. Finally, the process is reversed and the patient is closed, as is well known in the art. Thus this method does not require the use of a stiffened arm to provide for
20 the further stabilization. Only the spreading of the paddles is used.

 In a further embodiment, the system may be further configured to feature paddles which do not feature suction ports for capturing tissue. Rather, in this embodiment, shown in **FIG. 41** frictional engagement only by the bottom surface of the paddles is used along with the spreading action to stabilize the tissue. All other
25 aspects of this embodiment may be the same as shown already above. In a further alternative of this design, the tissue-contacting bottom surfaces of the paddles may be treated with materials or textures or both to enhance the friction or gripability between the tissue and the paddle. These embodiments may thus be used to perform a method of performing a surgical procedure upon a patient along the following steps of. First ,
30 a desired area of tissue on a patient is

accessed. Next, a stabilization system having an articulating arm, the articulating arm having a first pod and a second pod is provided. Preferably one or more of the pods has a bottom surface shaped to conform to the surface of the heart, and further the tissue-contacting bottom surfaces of the paddles are treated with materials or textures
5 or both to enhance the friction. Next the stabilization system is placed upon the surface of the tissue. Next the first pod and the second pod are spread relatively apart. Next the desired surgical procedure is performed. Thereafter the system is removed and the patient is closed.

In a still further embodiment, shown here in **FIG. 42**, the bottom surface may
10 feature a series of burrs or upraised barbs 656. These structures act as cleats which puncture or are introduced a small amount, between 0.25 to 1.5 millimeter beyond the surface of the tissue and into the tissue itself, more or less, and serve to enhance the friction or gripability between the tissue and the paddle. Moreover, still further, these structures may be made hollow and may be coupled to a dispensing reservoir
15 containing drugs, agents or other desired medicinal substance (such as anti-clotting agents, clotting agents, steroids, anti-biotics, growth factors, genetically acting agents or anti arrhythmic agents, to name only a few) so as to also be used to inject directly such substances into the tissue in the vicinity adjacent the surgical procedure, e.g. into the epicardium in the vicinity adjacent the anastomosis. Other than these features, all
20 other aspects of this embodiment may be the same as shown already above.

FIG. 43 is a perspective view of an alternative embodiment for tightening/spreading mechanism 21. In this embodiment a series of spreadable
wedges having a series of inclines which cooperate with a cable stop to provide a system wherein movement of the pos or paddles may be caused to occur concurrent
25 with or following arm tightening. As seen cable stop 300 is positioned at the distal end of arm. Cable stop hold the distal end of cable, not seen in this **FIG.** Cable stop is generally a cube like structure, having a relatively sharp corner or edge which is disposed to ride along first inclined surface 303 or second inclined surface 305 of spreadable saddle 307. As seen first inclined surface 303 is disposed at a first angle
30 on spreadable saddle while second inclined surface 305 is disposed at a second angle on spreadable saddle such that the first angle is relatively more flat or oblique in

regards to the bottom surface of cable stop 300 when compared to the second angle. Through these inclines and their angular relation to the bottom surface and side edges of cable stop, the co-efficient of friction between the cable stop and the first inclined surface 303 and second inclined surface 305 will be different. In such a manner, a first tension to the cable will generally first cause the arm and its links to be pulled together, thereafter, once tension exceeds the required coefficient of friction and cable stop is moved to engage the second inclined surface will the spreadable saddle be caused to fully begin to spread. As can be seen, a hemispherical mounting 309 is disposed between saddle 307 and U-link 311 such that spreading of saddle pinches mounting and therefore causes movement of the attached pods or paddles (only one of which is depicted here in outline as 22.)

FIG. 44 is a perspective view of an alternative embodiment for tightening/spreading mechanism 21. In this embodiment spread or other movement of the pods or paddles may be accomplished through hydraulic actuation. While shown here as hydraulic actuation, it should also be understood, as used herein, hydraulic also encompasses pneumatic actuation as well. As seen mechanism 21 features a spherical center hinge 400, which is used to couple the shown assembly to an articulated arm, as already described above. That is spherical center hinge 400 may be used in place of split ball. Left pod assembly 402 features a conventional connection 25 to permit suction to attached and communicated to a series of ports, as already described above. This embodiment further features a hydraulic actuator composed of the shaft 404 and seals 406, where the shaft is dimensioned to be slideably moved within runway 408 of left pod assembly. Stop 410 prevents excessive movement of shaft. While shaft itself is depicted as straight, it should be understood it could also be curved so that the right pod or paddle may be made to move in an arc. Runway 408 is coupled by a coupling 411 to hydraulic line 412, which in turn, is coupled to control valve 414 and hydraulic/pneumatic source 416.

FIG. 45 is a still further embodiment of the present invention. In this embodiment all other features are the same as those described above in regards to **FIG. 1** but for that the arm 420 is rigid, as opposed to the flexible arm shown above in **FIG. 1**. Rigid arm 420 may be used where the area in which the procedure is

performed is extremely cramped. Arm 420, because it does not flex may have a much decreased diameter as compared to arm 20 (recall that the FIGS. are not necessarily to scale.)

The present invention provides the following advantages over conventional suction stabilization systems. First, it reduces the force required to tighten and loosen the articulating arm(s). Second, it improves access to the surgical site in general due to its reduced size, and to the anastomosis site in particular due to the flexibility of the system components and geometry of the system components. Third, it permits relatively delicate manipulations to smoothly spread the suction pods without causing the suction pods to become detached from the arm. Fourth, use of a single arm to support multiple suction pods eliminates interference between opposing arms, such as occurred in the conventional systems when the surgeon tried to position the tissue stabilizers. Fifth, the time to set up the equipment is significantly reduced. Sixth, the design reduces inconsistent performance due to improper maintenance, wear, or unreliable mounting surfaces.

As disclosed, the present invention relates to a method and apparatus for immobilizing tissue. In the preferred embodiment, the invention is used to immobilize heart tissue for a coronary artery bypass graft procedure using either an open or closed chest approach, without the need for a cardiopulmonary bypass. Other surgical techniques, however, which require immobilizing body tissue may also be performed using the present invention, such as surgery on other organs such as the stomach, gall bladder, etc., as well as on other body tissues, such as the eye or the skin, for example. In addition, while the present invention has been described in detail with particular reference to a preferred embodiment and alternative embodiments, it should be understood variations and modifications can be effected within the scope of the following claims. Such modifications may include substituting elements or components which perform substantially the same function in substantially the same way to achieve substantially the same result for those described herein.

WHAT IS CLAIMED IS

1. A system for temporarily immobilizing an area of tissue comprising
a paddle assembly, paddle assembly having a first paddle and a second paddle,
the paddle assembly further having means for spreading the first paddle away from
5 the second paddle;
an arm having a distal end and a proximal end, the distal end coupled to the
paddle assembly, the arm having means for permitting the arm to flex, the arm having
means for fixing the arm to an object; and
arm locking means coupled to the arm, the arm locking means permitting the
10 locking of the arm in any selected position wherein the distal end of the arm is
maintained in the selected position.
2. The system according to claim 1 wherein the first paddle has means for
engaging heart tissue.
3. The system according to claim 2 wherein the means for engaging heart tissue
15 further comprises at least a first suction port positioned along a first surface of the
first paddle.
4. The system according to claim 3 wherein the means for engaging heart tissue
further comprises at least a second suction port positioned along a second surface of
the second paddle.
- 20 5. The system according to claim 4 wherein the first surface and the second
surface are generally within the same plane.
6. The system according to claim 5 further comprising the first paddle is adapted
to have a first surface which conforms to the surface of the heart.
7. The system according to claim 2 wherein the means for engaging heart tissue
25 further comprising a series of ridges along the first paddle lower surface.
8. The system according to claim 1 further comprising the first paddle is adapted
to have a first surface which is conformable to the surface of the heart.
9. The system according to claim 8 wherein the first paddle is constructed of a
malleable material.
- 30 10. The system according to claim 9 wherein the first paddle further comprises a
stiffening element therein.

11. The system according to claim 10 further comprising at least a first suction port positioned along a first surface of the first paddle.
12. The system according to claim 1 wherein the first paddle has at least one first suction port and the second paddle has at least one second suction port.
- 5 13. The system according to claim 12 further comprising a suction source.
14. The system according to claim 13 wherein the first paddle has means for coupling the at least one first suction port to the suction source.
15. The system according to claim 14 wherein the means for coupling are positioned along a proximal end of the first paddle.
- 10 16. The system according to claim 12 wherein the means for coupling further comprising a first nozzle adapted to be inserted into a polymeric tube.
17. The system according to claim 12 wherein the means for spreading comprises:
a cable stop coupled to distal end of arm, the arm having a cable running
therethrough, a distal end of cable coupled to cable stop, a spreadable saddle coupled
15 to distal end of arm, the spreadable saddle having a first inclined surface, wherein the cable stop will slide upon the first inclined surface as the cable receives a first amount of tension and the spreadable saddle is spread a first amount.
18. The system according to claim 17 wherein the spreadable saddle further comprises a second inclined surface, wherein the cable stop will slide upon the second
20 inclined surface as the cable receives a second amount of tension and the spreadable saddle is spread a second amount.
19. The system according to claim 17 further comprising a link disposed upon the distal end of the arm such the link is mounted between the arm and the saddle, a paddles mounting disposed between the link and the saddle.
- 25 20. The system according to claim 12 wherein the cable stop further comprises a generally cube like structure.
21. The system according to claim 20 wherein the means for spreading the first paddle and second paddle apart further comprises a hydraulic cylinder disposed upon the distal end of the arm, the first pod mounted to a first end of a first shaft couple to
30 the hydraulic cylinder and the second pod mounted to a second shaft coupled to the second end of the cylinder.

22. The system according to claim 21 further comprising a hydraulic reservoir and valve, the reservoir and valve providing hydraulic actuation of the hydraulic cylinder wherein the first paddle may be made to move relative to the second paddle through movement of hydraulic fluid from the hydraulic reservoir to the hydraulic cylinder.

5 23. The system according to claim 22 wherein the second shaft is curved wherein movement of the second paddle relative to the first paddle occurs in an arc.

24. The system according to claim 1 wherein the means for spreading further comprise means for independently spreading the first paddle and second paddle apart.

10 25. The system according to claim 24 wherein the means for independently spreading the first paddle and second paddle apart in a generally parallel relation are positioned upon the distal end of the arm.

26. The system according to claim 25 wherein the means for independently spreading the first paddle and second paddle apart further comprising a spreader (wheel), the spreader having a first screw, the first screw engaging with a first threaded hole in the first pod wherein movement of the spreader causes the first paddle to be moved in an axial direction along the first screw.

15 27. The system according to claim 26 further comprising the spreader having a second screw, the second screw engaging with a second threaded hole in the second pod wherein movement of the spreader causes the second paddle to be moved in an axial direction along the second screw.

20 28. The system according to claim 26 further comprising the spreader having a second screw, the second screw engaging with a second threaded hole in the second pod wherein movement of the spreader causes the second paddle to be moved in direction parallel to the first paddle.

25 29. The system according to claim 24 further comprising a first means for biasing the first paddle away from the spreader, the means for biasing disposed adjacent the first paddle.

30. The system according to claim 29 wherein the first means for biasing the first paddle away from the spreader further comprises a torsion spring disposed about the first screw so as to bias the first paddle away from the spreader.

5 31 The system according to claim 29 further comprising a second means for biasing the first paddle away from the spreader, the means for biasing disposed adjacent the first paddle.

32. The system according to claim 31 wherein the second means for biasing the first paddle away from the spreader.

10 33 The system according to claim 31 further comprising a torsion spring disposed about the second screw so as to bias the first paddle away from the spreader.

34. The system according to claim 1 wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle a parallel relation.

15 35. The system according to claim 1 wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle in a non parallel relation.

36. The system according to claim 1 wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge.

20 37. The system according to claim 36 wherein the spreadable hinge is coupled to the arm locking means.

38. The system according to claim 37 wherein the spreadable hinge is coupled to the arm locking means by a cable wire.

39. The system according to claim 38 wherein the cable is stranded.

40. The system according to claim 37 wherein the spreadable hinge further comprising a split ball, a first end of the split ball coupled to the first paddle, a second end of the split ball coupled to the split ball.

5 41. The system according to claim 40 wherein the split ball is adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the split ball is dimension to be pressured by the sling in the second position, the split ball having a split, the split ball and split further sized to be compressed due to the force exerted upon it by the sling.

10 42. The system according to claim further comprising a head link positioned at the distal end of the arm wherein the split ball is adapted to be mated into the retention sling and against the head link.

43. The system according to claim 40 wherein the split ball has a split, the split symmetrical about a first plane.

15 44. The system according to claim 43 wherein the split ball has a split, the split symmetrical about a second plane.

45. The system according to claim 44 wherein the split ball has a split, the split symmetrical about a first plane which is non-parallel to a major plane of the paddle assembly.

20 46. The system according to claim wherein 1 the means for spreading the first paddle and second paddle apart further comprising a segmented spreadable hinge.

47. The system according to claim 46 wherein the segmented spreadable hinge is coupled to the arm locking means.

48. The system according to claim 47 wherein the segmented spreadable hinge further comprises a intermating ball and socket assembly.

49. The system according to claim 48 wherein the intermating ball and socket assembly further comprises a first ball having a first end and a hemisphere having a second end, the first end of the first ball coupled to the first paddle, the second end of the hemisphere coupled to the second paddle.

50. The system according to claim 49 wherein the hemisphere has a hollow, the first end of the first ball is sized to be mated into the hollow.

51. The system according to claim 50 wherein the first ball mated into the hemisphere are further adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the first ball and the hemisphere are dimension to be pressured by the sling in the second position wherein the first ball rotates relative to the hemisphere.

52. The system according to claim 51 further comprising a head link positioned at the distal end of the arm wherein the first ball and the hemisphere are adapted to be positioned into the retention sling and against the head link.

53. The system according to claim 1 wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart.

54. The system according to claim 53 further comprising means for simultaneously rotating the first paddle along its first major axis in a first direction.

55. The system according to claim 54 further comprising means for simultaneously rotating the second paddle along its second major axis in a second direction.

56. The system according to claim 55 wherein the first direction is opposite the second direction.

57. The system according to claim 1 wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position, wherein in the first position the first paddle and second paddle are configured in a parallel relation.

58. The system according to claim 57 wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position, wherein in the second position the first paddle and second paddle are configured in a parallel relation.

5 59. The system according to claim 1 wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position.

60. The system according to claim 59 wherein in the first position the first paddle and second paddle are configured in a non parallel relation.

10 61. The system according to claim 60 wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position.

62. The system according to claim 60 wherein in the second position the first paddle and second paddle are configured in a non parallel relation.

15 63. The system according to claim 1 wherein the first paddle has a first surface, a first suction port positioned within the first surface, a second suction port positioned within the first surface, a third suction port positioned within the first surface.

64. The system according to claim 63 wherein the first suction port, the second suction port, and the third suction port are all in a linear relation.

20 65. The system according to claim 64 further comprising a suction source, the first suction port coupled to the suction source through a first suction aperture, the first suction aperture having a first suction aperture surface area.

66. The system according to claim 65 further comprising a suction source, the second suction port coupled to the suction source through a second suction aperture, the second suction aperture having a second suction aperture surface area.

25 67. The system according to claim 66 further comprising a suction source, the third suction port coupled to the suction source through a third suction aperture, the third suction aperture having a third suction aperture surface area.

68. The system according to claim 66 wherein the first suction aperture surface area is different from the second suction aperture surface area.

30 69. The system according to claim 68 wherein the third suction aperture surface area is different from the second suction aperture surface area.

70. The system according to claim 64 wherein the first suction port has a non-circular shape within the first plane.

71. The system according to claim 64 wherein the non-circular shape within the first plane is an ellipse.

5 72. The system according to claim 64 wherein the non-circular shape within the first plane is a trapezoid.

73. The system according to claim 64 wherein the non-circular shape within the first plane is a square.

74. The system according to claim 64 wherein the first suction port is larger than
10 the second suction port.

75. The system according to claim 74 wherein the first suction port is disposed closer to the proximal end of the first paddle than the second suction port.

76. The system according to claim 75 wherein the second suction port is larger
than the third suction port.

15 77. The system according to claim 75 wherein the second suction port is smaller than the third suction port.

78. The system according to claim 1 wherein the first paddle has a rectangular cross section along a first plane.

79. The system according to claim 1 wherein the first paddle has a triangular cross
20 section along a first plane.

80. The system according to claim 1 further comprising the first paddle has a first surface, a first suction port positioned within the first surface, a suction source, the first suction port coupled to the suction source through a first suction aperture, the first suction port having a bottom opening within the first surface and an upper
25 surface within the first paddle, the suction aperture positioned within the first paddle between the first surface of the first paddle and the upper surface of the first suction port.

81. The system according to claim 1 wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first
30 paddle and second paddle apart.

82. The system according to claim 1 wherein the arm has a series of articulations wherein the arm may be bent along a curved arc among a plurality of direction.

83. The system according to claim 82 wherein the series of articulations are provided through a series of interlocking links.

5 84. The system according to claim 83 wherein at least one first link in the series of interlocking links has a first hemispherical surface having a first hemispherical diameter and at least one second link in the series of interlocking links has a second hemispherical indentation having a second hemispherical diameter.

10 85. The system according to claim 84 wherein the first diameter is equal to the second diameter.

86. The system according to claim 85 wherein the at least one first link has a first center lumen therethrough and the at least one second link has a second center lumen therethrough, the first link and the second link coupled through a first tensioning element disposed within the respective center lumens.

15 87. The system according to claim 1 wherein the means for spreading the first paddle away from the second paddle further comprises a tensioning element running from a proximal end of the arm to the distal end of the arm.

88. The system according to claim 87 wherein the cable running from a proximal end of the arm to the distal end of the arm is a stranded cable.

20 89. The system according to claim 1 wherein the arm comprises a series of interlocking links, each link having a hemispherical protrusion and a hemispherical indentation.

90. The system according to claim 89 wherein the links are constructed from a polymer.

25 91. The system according to claim 90 wherein the polymer comprises a glass fiber filled thermoplastic.

92. The system according to claim 91 wherein a surface of the hemispherical protrusion and a surface of the hemispherical indentation has a roughened texture.

30 93. The system according to claim 89 wherein a surface of the hemispherical protrusion and a surface of the hemispherical indentation has a series of interlocking dimples and depressions.

94. The system according to claim 1 wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed on the proximal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.

5 95. The system according to claim 94 wherein the spreading actuator further comprises a torque screw.

96. The system according to claim 1 wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed away from the distal end of the arm, while the first paddle and second paddle are disposed
10 on the distal end of the arm.

97. The system according to claim 96 wherein the spreading actuator further comprises a torque screw.

98. The system according to claim 96 wherein the spreading actuator further comprises a hydraulic reservoir.

15 99. The system according to claim 89 wherein the first hemispherical surface has a series of first protrusions of a first protrusion shape.

100. The system according to claim 99 wherein the second hemispherical indentation has a series of second indentations of a second indentation shape.

101. The system according to claim 100 wherein the first protrusions are
20 substantially the same size as the second indentations.

102. The system according to claim 100 wherein the first hemispherical surface has a series of first indentations of a first indentations shape.

103. The system according to claim 100 wherein the second hemispherical indentation has a series of second protrusions of a second protrusions shape.

25 104. The system according to claim 1 wherein the first paddle having a first bottom surface shaped to engage the surface of the tissue.

105 The system according to claim 104 wherein the first bottom surface further comprises a series of tissue puncturing cleats.

106 The system according to claim 105 wherein the series of tissue puncturing
30 cleats extend for a distance between 0.25 and 1.0 millimeter from the first bottom surface.

107 The system according to claim 105 wherein the series of tissue puncturing cleats are hollow.

108 The system according to claim 107 wherein the series of tissue puncturing cleats are coupled to a dispensing reservoir.

5 109 The system according to claim 108 wherein the dispensing reservoir contains a medicinal substance.

110. A system for stabilizing tissue comprising

a paddle assembly, paddle assembly having a first paddle and a second paddle, the paddle assembly further having means for spreading the first paddle away from the second paddle; and

10

an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm having means for permitting the arm to flex, the arm having means for fixing the arm to an object.

111. The system according to claim 110 further comprising arm locking means coupled to the arm, the arm locking means permitting the locking of the arm in any selected position wherein the distal end of the arm is maintained in the selected position.

15

112. The system according to claim 111 wherein the first paddle has means for engaging heart tissue.

20 113. The system according to claim 112 wherein the means for engaging heart tissue further comprises at least a first suction port positioned along a first surface of the first paddle.

114. The system according to claim 113 wherein the means for engaging heart tissue further comprises at least a second suction port positioned along a second surface of the second paddle.

25

115. The system according to claim 114 wherein the first surface and the second surface are generally within the same plane.

116. The system according to claim 115 further comprising the first paddle is adapted to have a first surface which conforms to the surface of the heart.

30 117. The system according to claim 110 wherein the first paddle has at least one first suction port and the second paddle has at least one second suction port.

118. The system according to claim 110 further comprising a suction source.

119. The system according to claim 118 wherein the first paddle has means for coupling the at least one first suction port to the suction source.

120. The system according to claim 119 wherein the means for coupling are
5 positioned along a proximal end of the first paddle.

121. The system according to claim 110 wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle a parallel relation.

122. The system according to claim 110 wherein the means for spreading the first
10 paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle in a non parallel relation.

123. The system according to claim 110 wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge.

124. The system according to claim 123 wherein the spreadable hinge is coupled to
15 the arm locking means.

125. The system according to claim 124 wherein the spreadable hinge is coupled to the arm locking means by a cable wire.

126. The System according to claim 125 wherein the cable is stranded.

127. The system according to claim 124 wherein the spreadable hinge further
20 comprising a split ball, a first end of the split ball coupled to the first paddle, a second end of the split ball coupled to the split ball.

128. The system according to claim 126 wherein the split ball is adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the split ball is dimension to be
25 pressured by the sling in the second position, the split ball further sized to be spread apart due to the force exerted upon it by the sling.

129. The system according to claim 127 further comprising a head link positioned at the distal end of the arm wherein the split ball is adapted to be mated into the retention sling and against the head link.

130. The system according to claim 110 wherein the split ball has a split, the split
30 symmetrical about a first plane.

131. The system according to claim 129 wherein the split ball has a split, the split symmetrical about a second plane.

132. The system according to claim 130 wherein the split ball has a split, the split symmetrical about a first plane which is non-parallel to a major plane of the paddle assembly.

133. The system according to claim 110 wherein the means for spreading the first paddle and second paddle apart further comprising a segmented spreadable hinge.

134. The system according to claim 110 wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart.

135. The system according to claim 133 further comprising means for simultaneously rotating the first paddle along its first major axis in a first direction.

136. The system according to claim 134 further comprising means for simultaneously rotating the second paddle along its second major axis in a second direction.

137. The system according to claim 135 wherein the first direction is opposite the second direction.

138. The system according to claim 110 wherein the first paddle and second paddle are located in a first position and may be spread apart to a second position, wherein in the first position the first paddle and second paddle are configured in a parallel relation.

139. The system according to claim 110 wherein the first paddle has a first surface, a first suction port positioned within the first surface, a second suction port positioned within the first surface, a third suction port positioned within the first surface.

140. The system according to claim 138 wherein the first suction port, the second suction port, and the third suction port are all in a linear relation.

141. The system according to claim 110 further comprising the first paddle has a first surface, a first suction port positioned within the first surface, a suction source, the first suction port coupled to the suction source through a first suction aperture, the first suction port having a bottom opening within the first surface and an upper surface within the first paddle, the suction aperture positioned within the first paddle

between the first surface of the first paddle and the upper surface of the first suction port.

142. The system according to claim 111 wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first paddle and second paddle apart.

143. The system according to claim 110 wherein the arm has a series of articulations wherein the arm may be bent along a curved arc among a plurality of direction.

144. The system according to claim 142 wherein the series of articulations are provided through a series of interlocking links.

145. The system according to claim 110 wherein the means for spreading the first paddle away from the second paddle further comprises a tensioning element running from a proximal end of the arm to the distal end of the arm.

146. A system for temporarily immobilizing an area of tissue comprising a paddle assembly, paddle assembly having a first paddle and a second paddle, the first paddle having a first bottom surface shaped to engage the surface of the tissue, the bottom surface having means to enhance the friction between the tissue and the paddle bottom surface, the paddle assembly further having means for spreading the first paddle away from the second paddle;

an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm having means for permitting the arm to flex, the arm having means for fixing the arm to an object; and

arm locking means coupled to the arm, the arm locking means permitting the locking of the arm in any selected position wherein the distal end of the arm is maintained in the selected position.

147. The system according to claim 145 the first paddle having a first bottom surface shaped to engage the surface of the tissue.

148. The system according to claim 145 the first bottom surface further comprises a series of tissue puncturing cleats.

149. The system according to claim 145 wherein the first paddle has means for engaging heart tissue.

150. The system according to claim 148 wherein the means for engaging heart tissue further comprises at least a first suction port positioned along a first surface of the first paddle.

5 151. The system according to claim 149 wherein the means for engaging heart tissue further comprises at least a second suction port positioned along a second surface of the second paddle.

152. The system according to claim 150 wherein the first surface and the second surface are generally within the same plane.

10 153. The system according to claim 150 further comprising the first paddle is adapted to have a first surface which conforms to the surface of the heart.

154. The system according to claim 145 wherein the means for spreading further comprise means for independently spreading the first paddle and second paddle apart.

155. The system according to claim 145 wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge.

15 156. The system according to claim 154 wherein the spreadable hinge is coupled to the arm locking means.

157. The system according to claim 154 wherein the spreadable hinge further comprising a split ball, a first end of the split ball coupled to the first paddle, a second end of the split ball coupled to the split ball.

20 158. The system according to claim 156 wherein the split ball is adapted to be mated into a retention sling, the retention sling moveable from a first, non-tensioned position to a second, tensioned position, wherein the split ball is dimension to be pressured by the sling in the second position, the split ball further sized to be spread apart due to the force exerted upon it by the sling.

25 159. The system according to claim 157 further comprising a head link positioned at the distal end of the arm wherein the split ball is adapted to be mated into the retention sling and against the head link.

160. The system according to claim 156 wherein the split ball has a split, the split symmetrical about a first plane.

30 161. The system according to claim 159 wherein the split ball has a split, the split symmetrical about a second plane.

162. The system according to claim 160 wherein the split ball has a split, the split symmetrical about a first plane which is non-parallel to a major plane of the paddle assembly.

163. The system according to claim 145 wherein the means for spreading the first paddle and second paddle apart further comprising a segmented spreadable hinge.

164. The system according to claim 145 wherein the arm has a series of articulations wherein the arm may be bent along a curved arc among a plurality of direction.

165. The system according to claim 163 wherein the series of articulations are provided through a series of interlocking links.

166. The system according to claim 164 wherein at least one first link in the series of interlocking links has a first hemispherical surface having a first hemispherical diameter and at least one second link in the series of interlocking links has a second hemispherical indentation having a second hemispherical diameter.

167. The system according to claim 145 wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed on the proximal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.

168. The system according to claim 145 wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed away from the distal end of the arm, while the first paddle and second paddle are disposed on the distal end of the arm.

169. A system for temporarily immobilizing an area of tissue comprising
a paddle assembly, paddle assembly having a first paddle and a second paddle,
the paddle assembly further having means for moving the first paddle relative to the
second paddle;

an arm having a distal end and a proximal end, the distal end coupled to the
paddle assembly, the arm having means for permitting the arm to flex, the arm having
means for fixing the arm to an object; and

arm locking means coupled to the arm, the arm locking means permitting the locking of the arm in any selected position wherein the distal end of the arm is maintained in the selected position.

5 170. The system according to claim 168 wherein the means for moving the first paddle relative to the second paddle further comprise means for spreading the first paddle away from the second paddle.

171. The system according to claim 169 wherein the means for spreading the first paddle and second paddle apart further comprises a spreading actuator disposed on the proximal end of the arm, while the first paddle and second paddle are disposed on the
10 distal end of the arm.

172. The system according to claim 170 wherein the spreading actuator is a torque screw.

173. The system according to claim 168 wherein the first paddle has means for engaging heart tissue.

15 174. The system according to claim 172 wherein the means for engaging heart tissue further comprises at least a first suction port positioned along a first surface of the first paddle.

175. The system according to claim 173 wherein the means for engaging heart tissue further comprises at least a second suction port positioned along a second
20 surface of the second paddle.

176. The system according to claim 175 wherein the first surface and the second surface are generally within the same plane.

177. The system according to claim 174 further comprising the first paddle is adapted to have a first surface which conforms to the surface of the heart.

25 178. A system for stabilizing tissue comprising
a paddle assembly, paddle assembly having a fist paddle and a second paddle, the paddle assembly further having means for spreading the first paddle away from the second paddle;

30 an arm having a distal end and a proximal end, the distal end coupled to the paddle assembly, the arm having means for fixing the arm to an object; and

means for spreading the first paddle and second paddle apart, the means for spreading coupled to a proximal end of the arm.

179. The system according to claim 177 wherein the first paddle has a first surface, a first suction port positioned within the first surface, a second suction port positioned
5 within the first surface, a third suction port positioned within the first surface.

180. The system according to claim 178 wherein the first suction port, the second suction port, and the third suction port are all in a linear relation.

181. The system according to claim 177 wherein the means for spreading further comprise means for independently spreading the first paddle and second paddle apart.

10 182. The system according to claim 177 wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first paddle away from the second paddle a parallel relation.

183. The system according to claim 177 wherein the means for spreading the first paddle away from the second paddle further comprising means for spreading the first
15 paddle away from the second paddle in a non parallel relation.

184. The system according to claim 177 wherein the means for spreading the first paddle and second paddle apart further comprising a spreadable hinge.

185. The system according to claim 177 wherein the arm locking means further comprising means for simultaneously activating the means for spreading the first
20 paddle and second paddle apart.

1 / 23

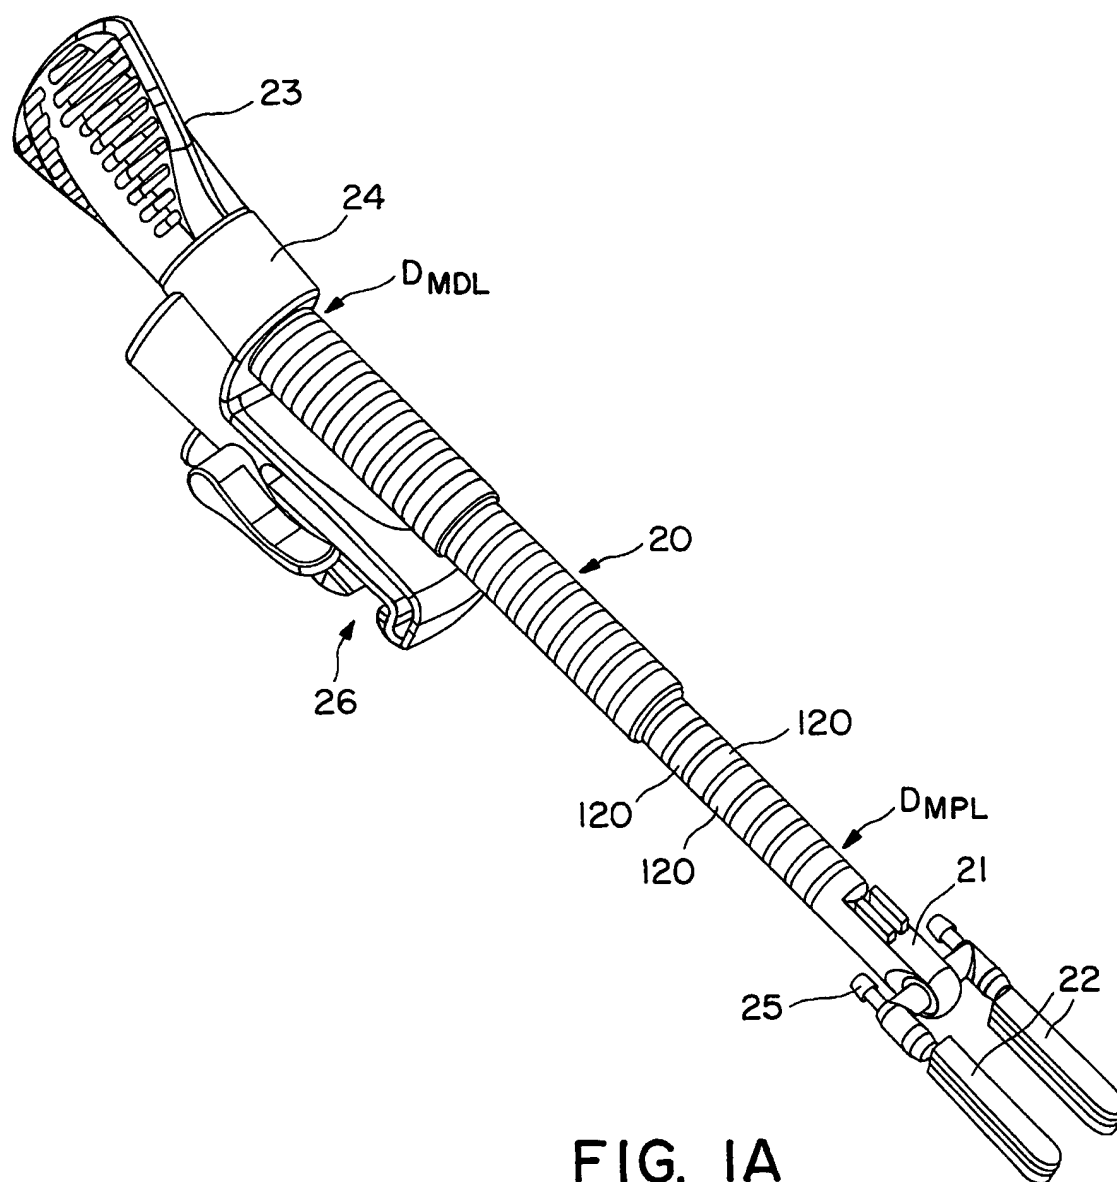


FIG. 1A

SUBSTITUTE SHEET (RULE26)

2/23

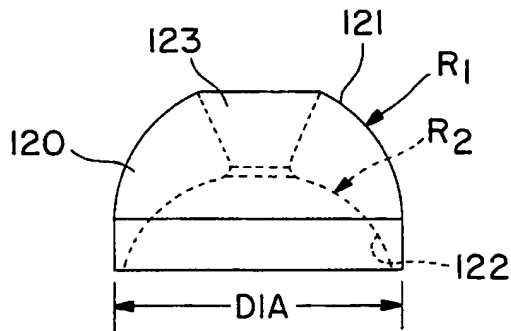


FIG. 1B

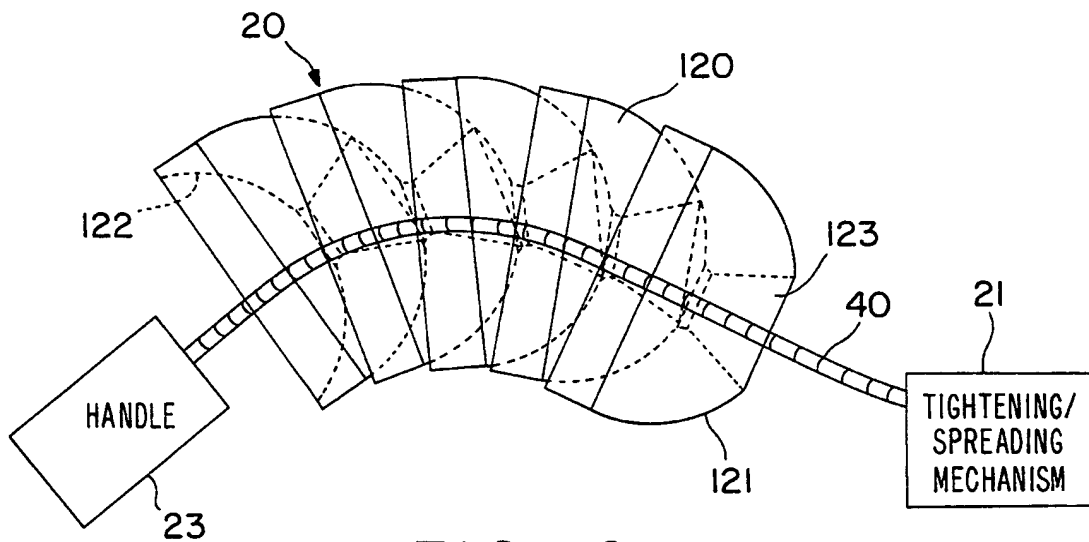


FIG. 1C

3 / 23

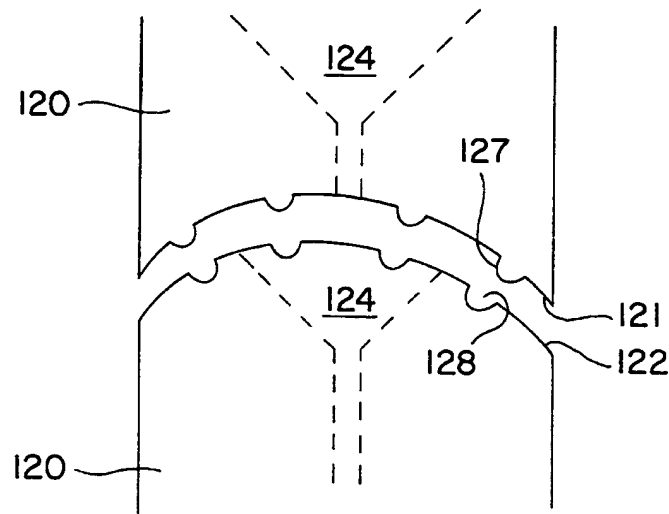


FIG. 1E

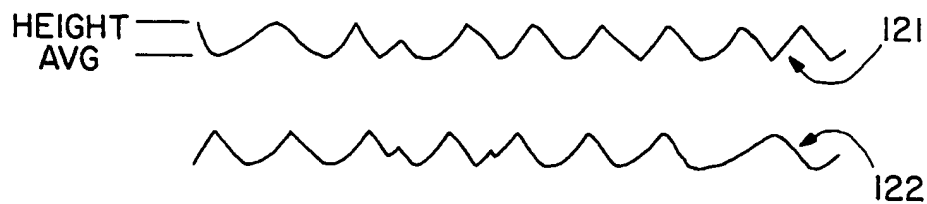


FIG. 1D

4/23

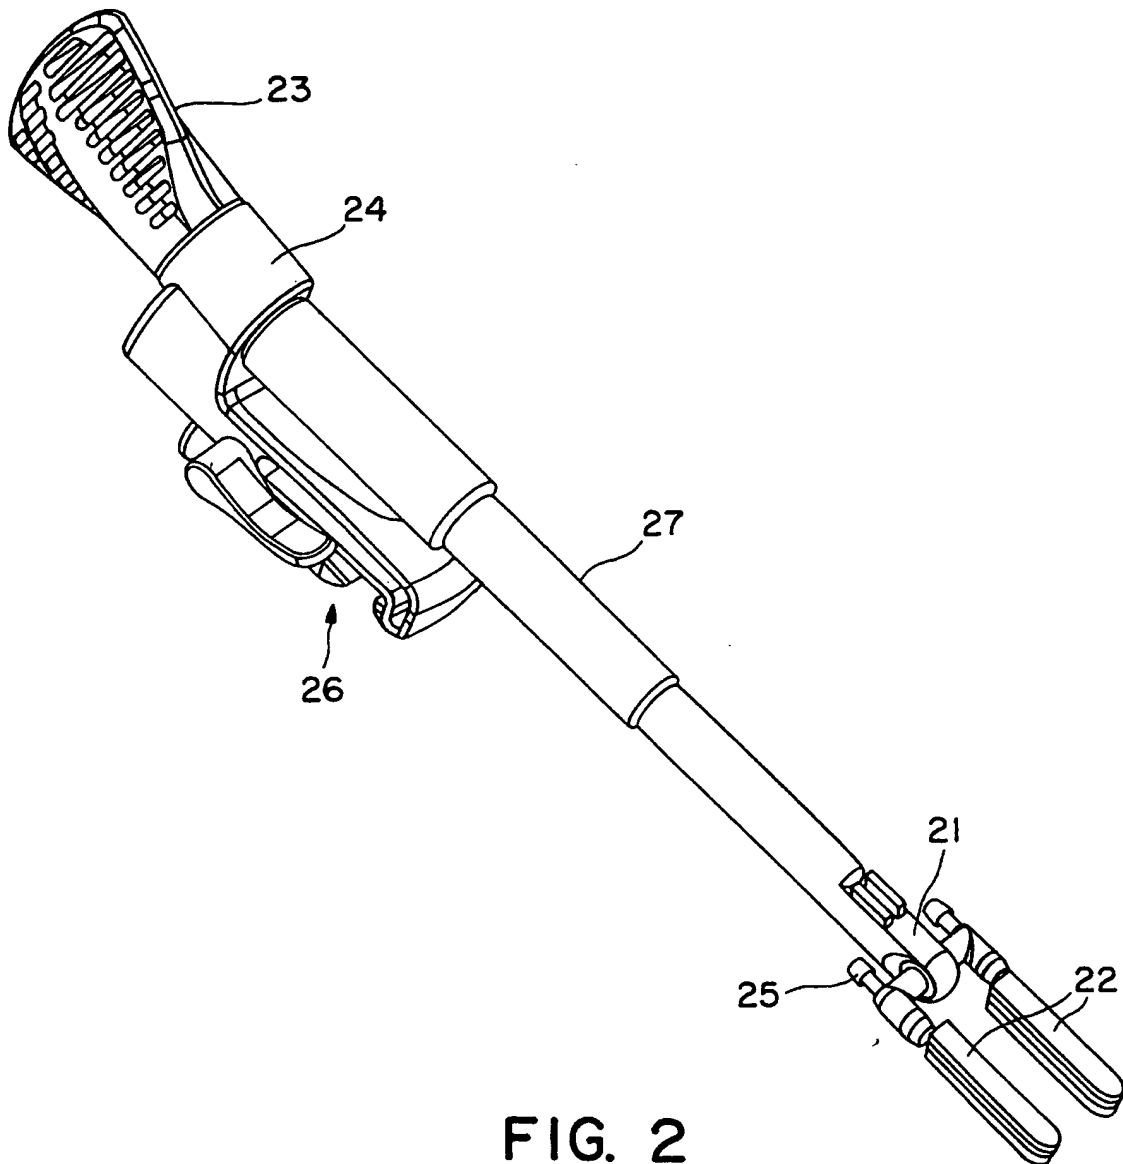


FIG. 2

5/23

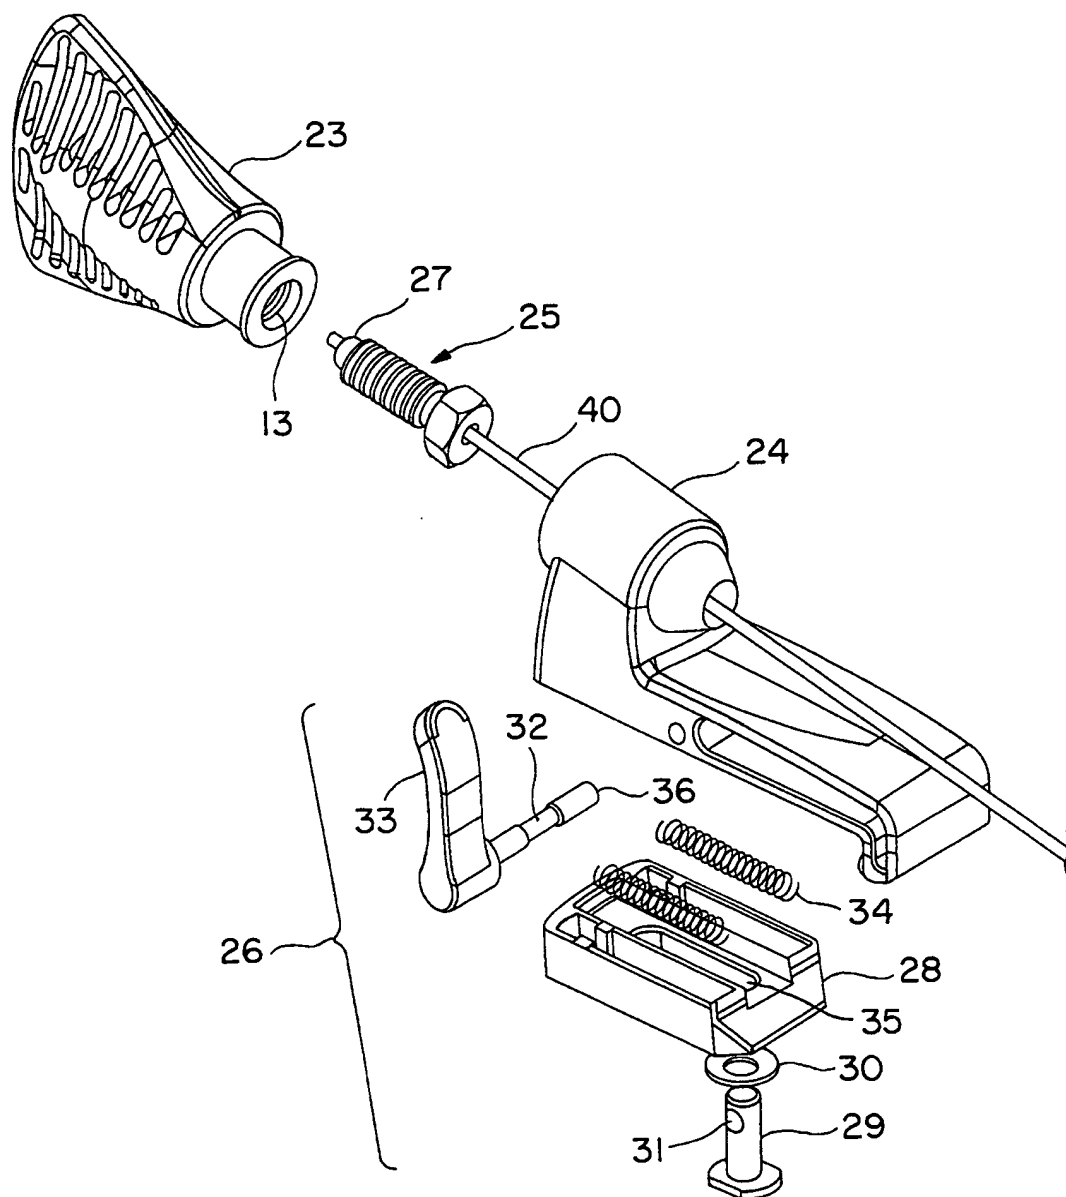


FIG. 3

6 / 23

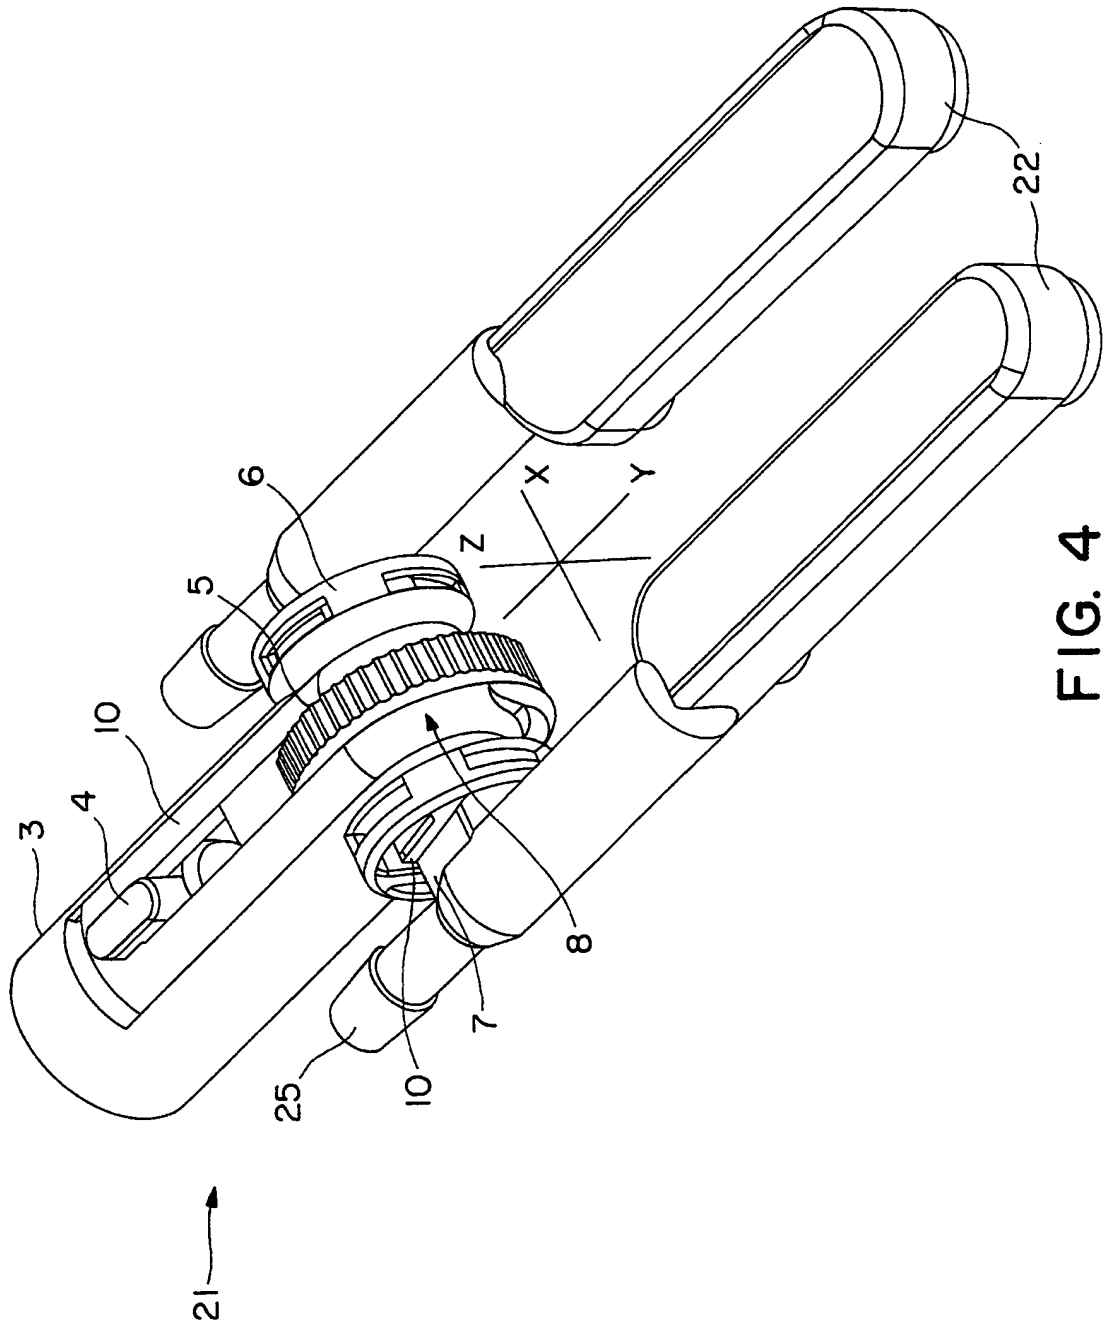


FIG. 4

7/23

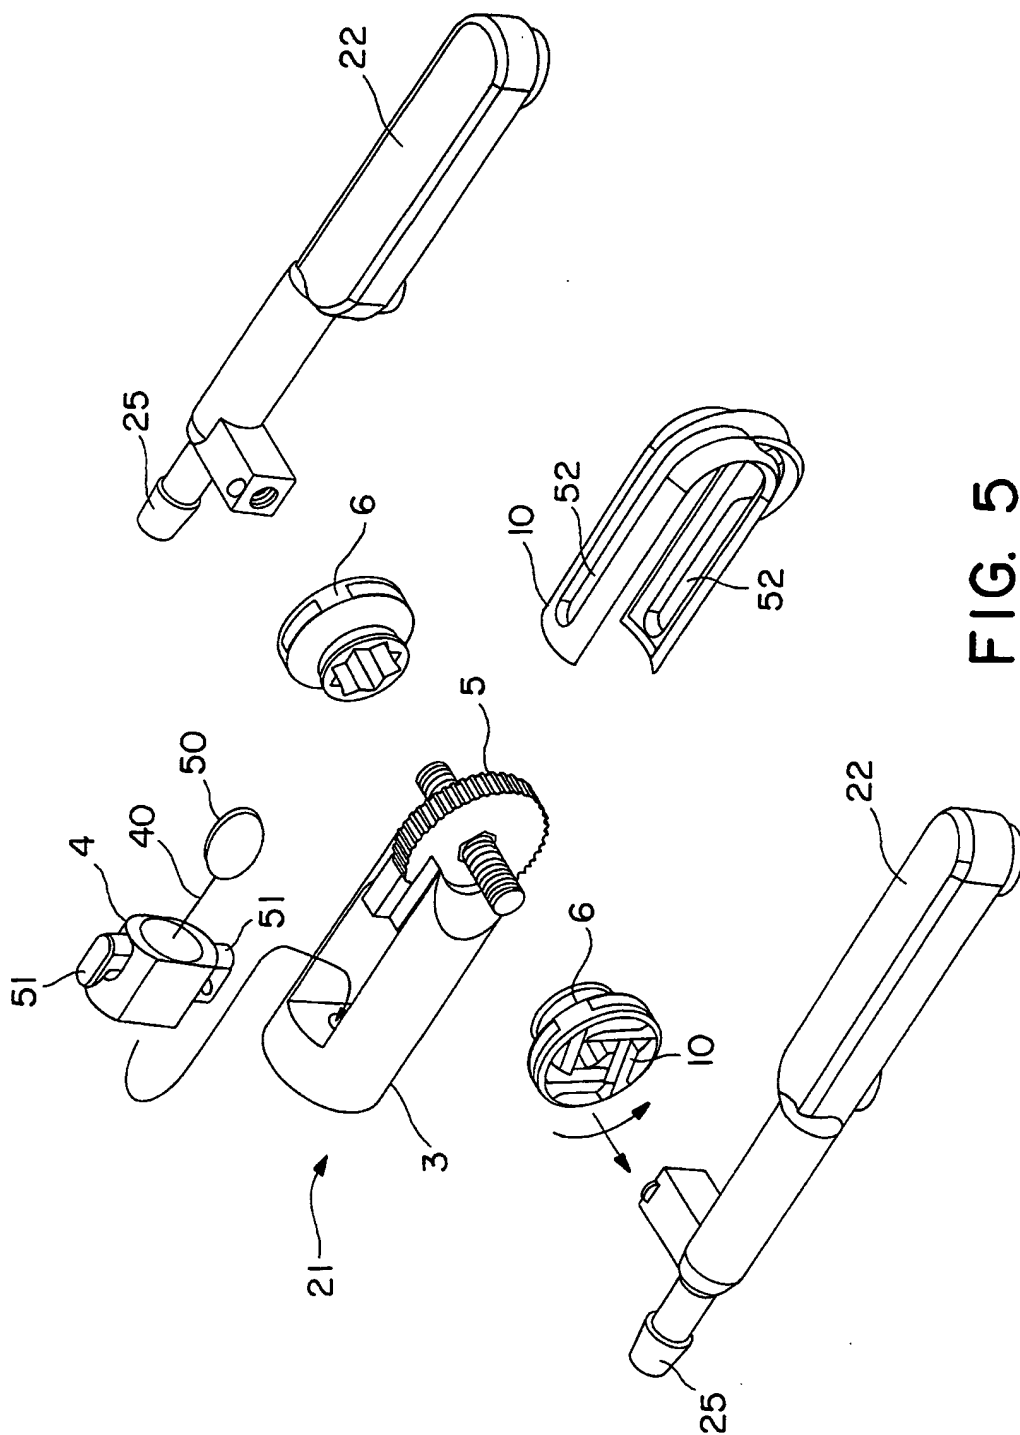


FIG. 5

9/23

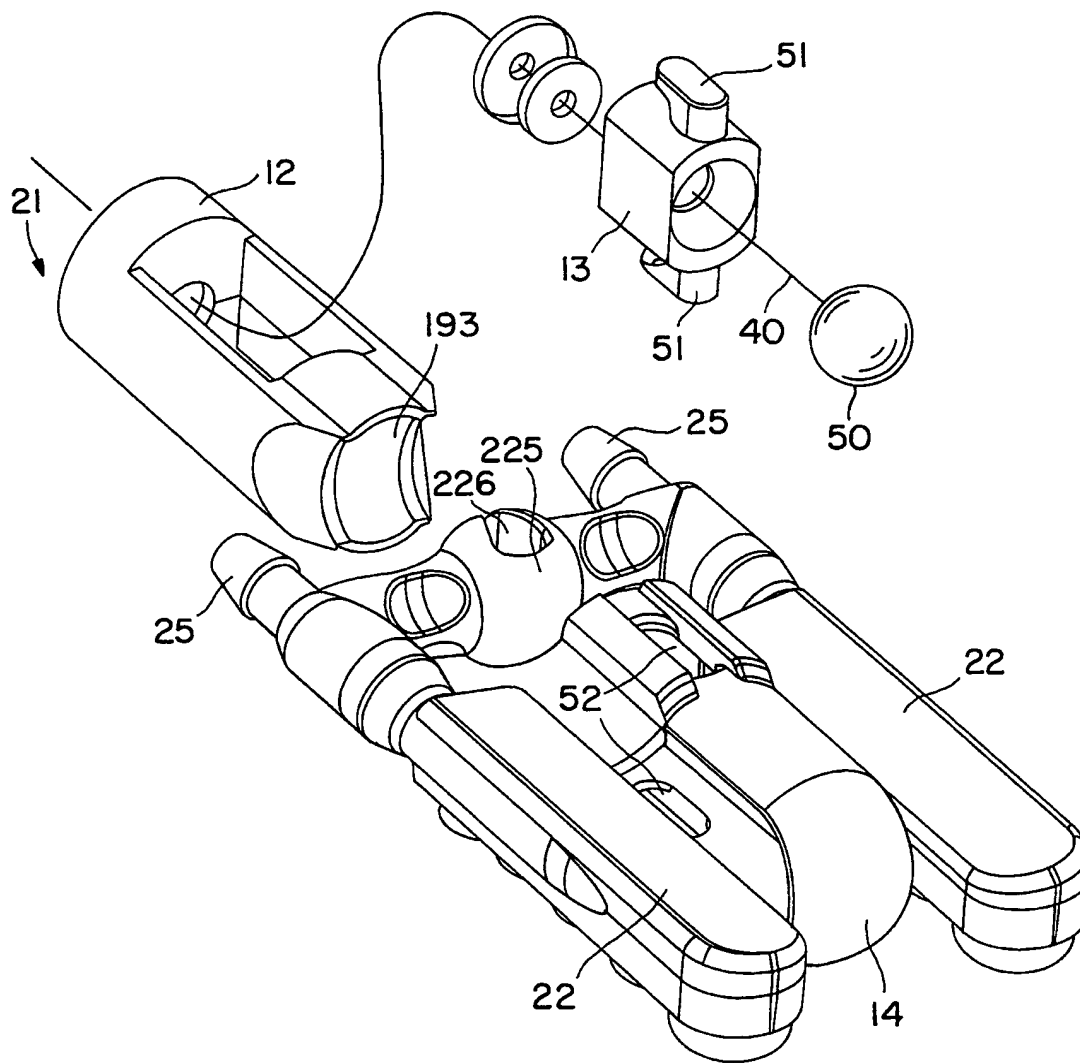


FIG. 7

10/ 23

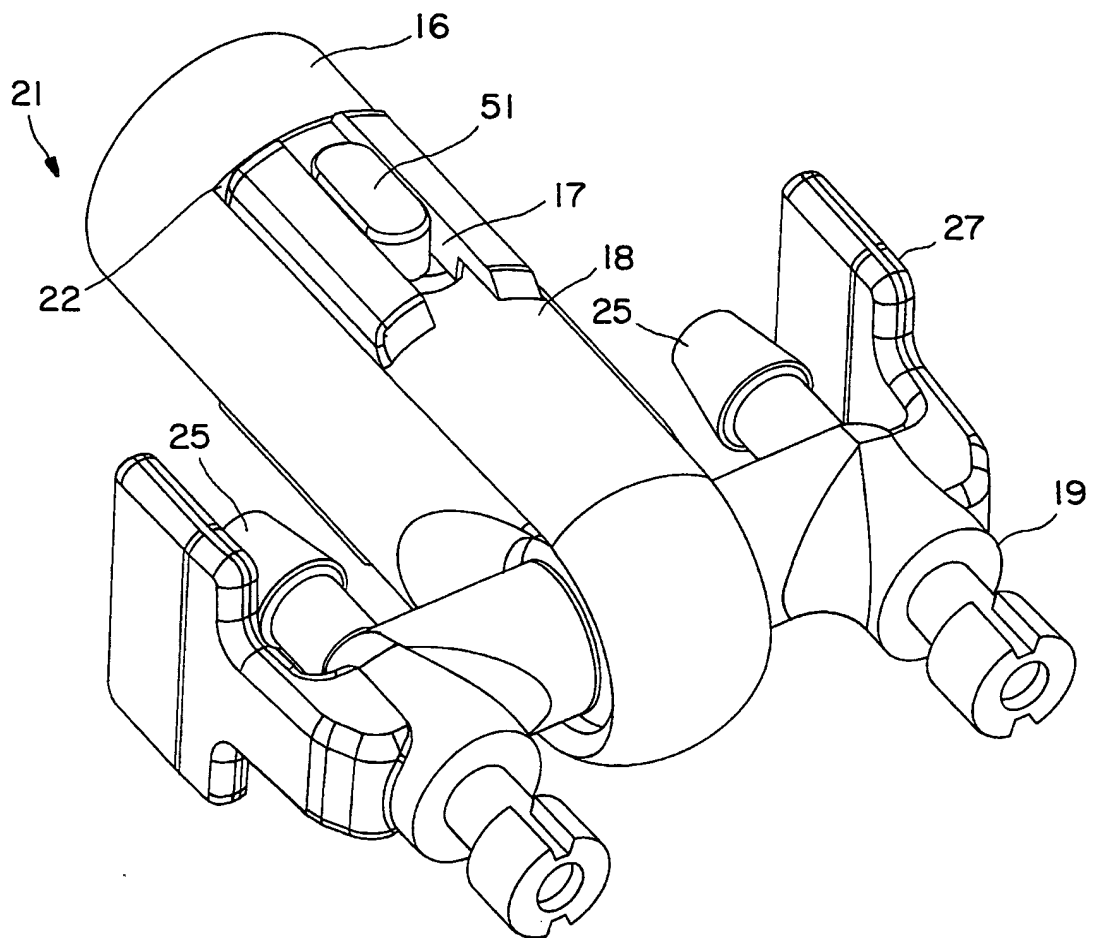


FIG. 8

11 / 23

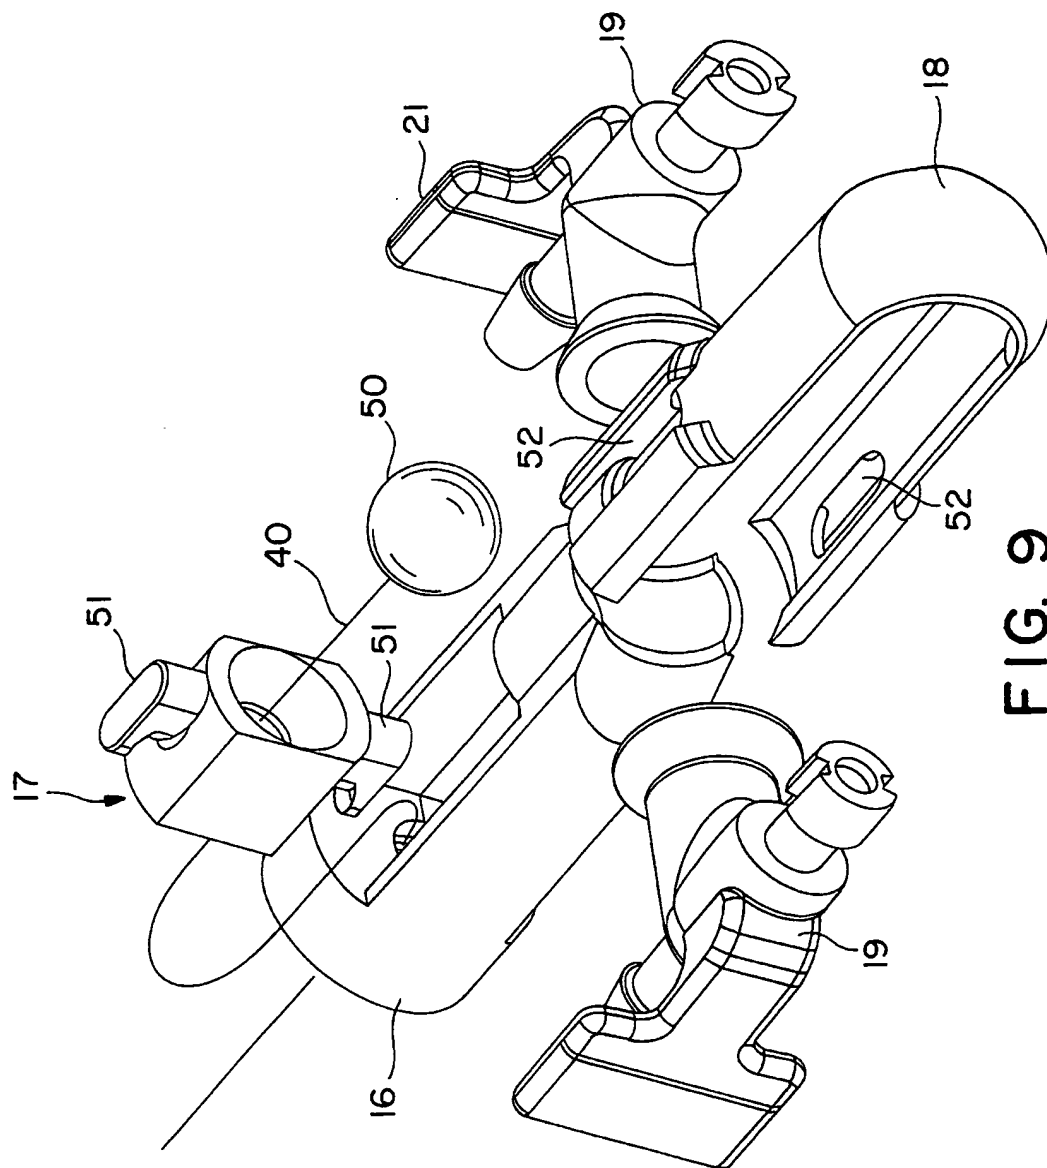


FIG. 9

12/23

STIFFNESS vs. SPREAD

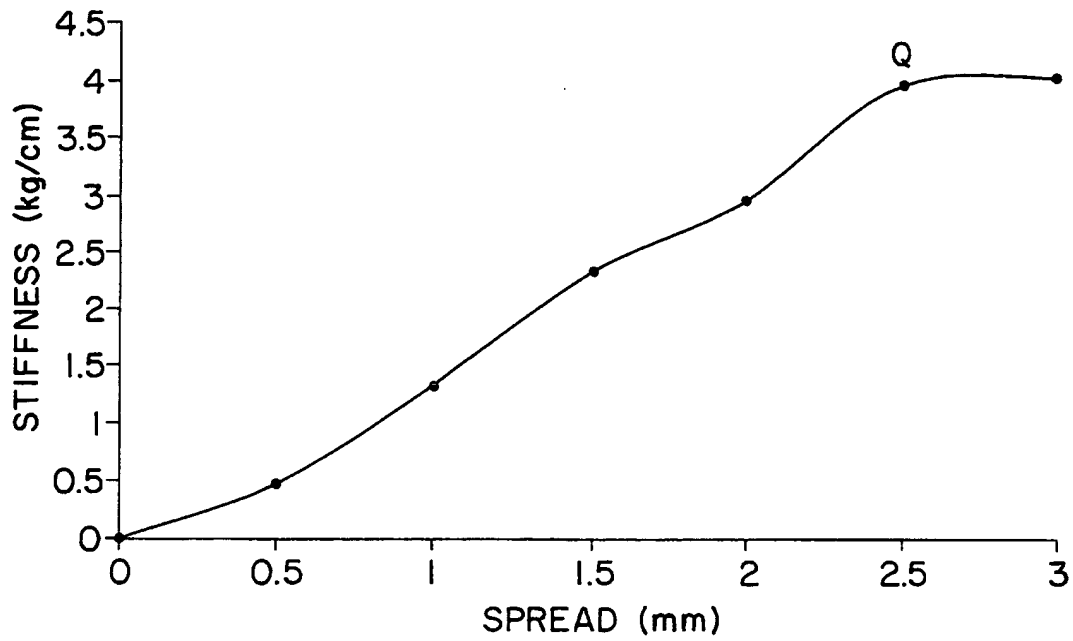


FIG. 10

RIGIDITY

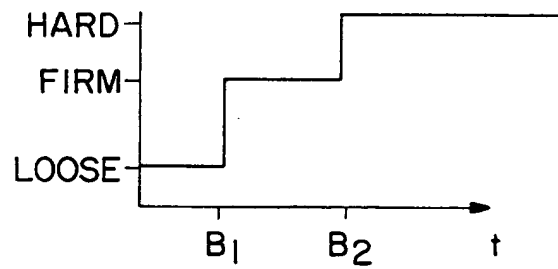


FIG. 11

SPREAD

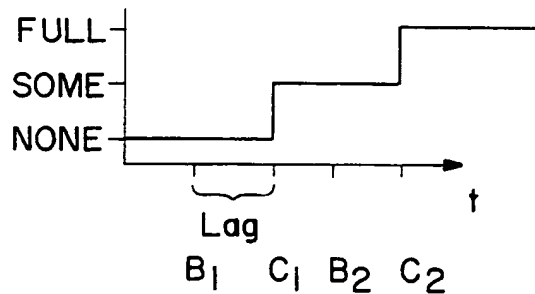


FIG. 12

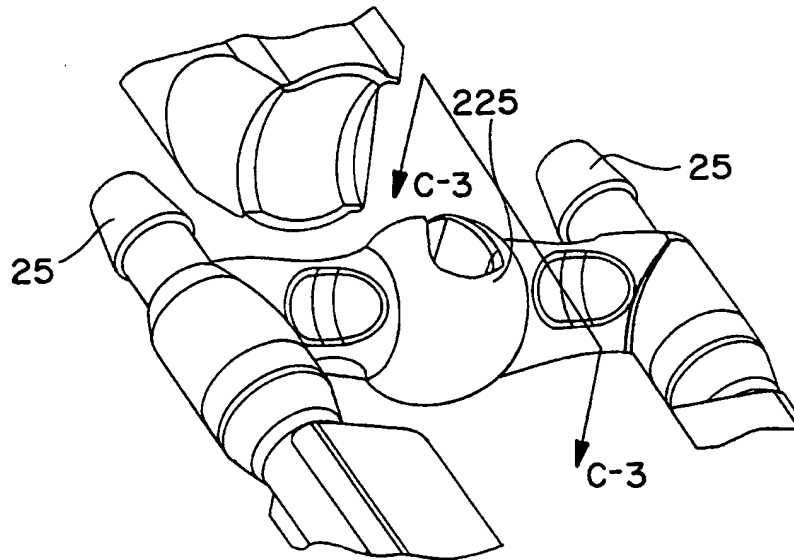


FIG. 13

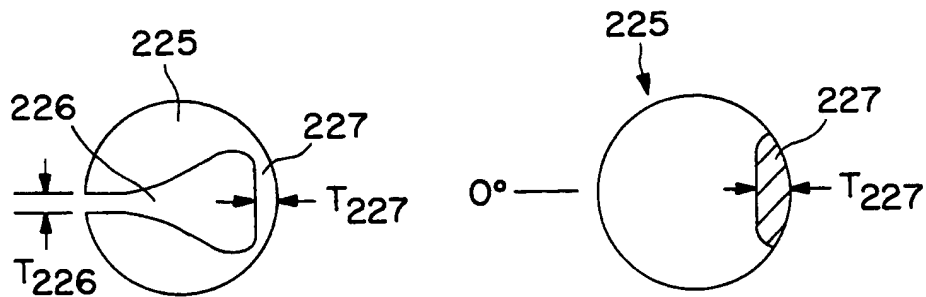


FIG. 14

FIG. 15

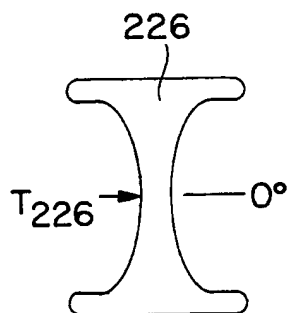


FIG. 16

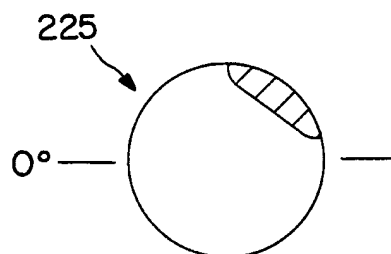


FIG. 17

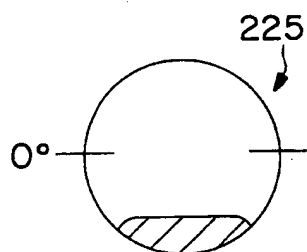


FIG. 18

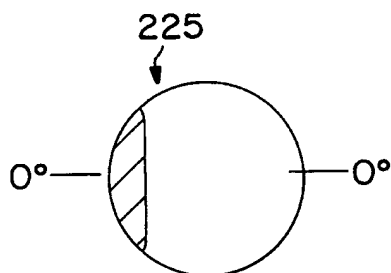


FIG. 19

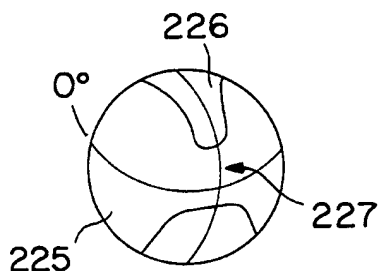


FIG. 20




FIG. 21

15/23

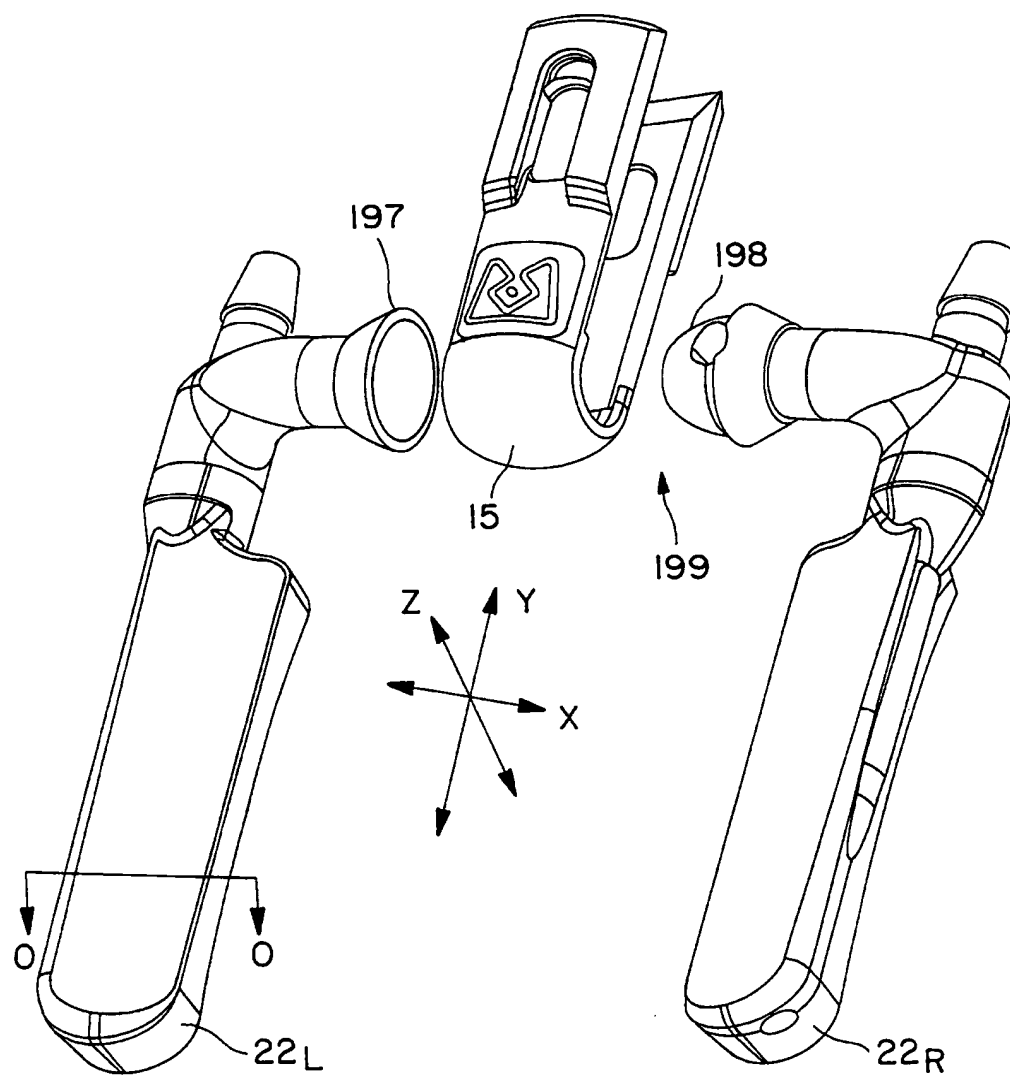


FIG. 22

16/23

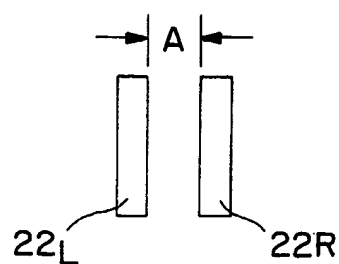


FIG. 23

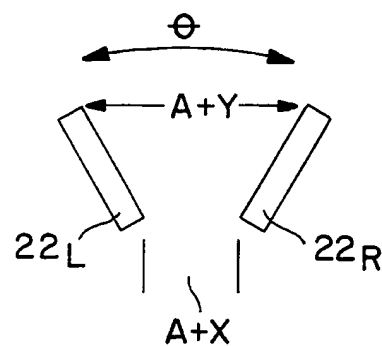


FIG. 24

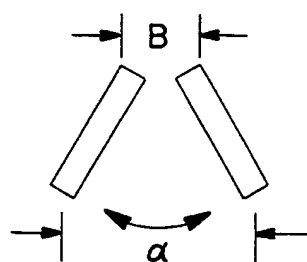


FIG. 25

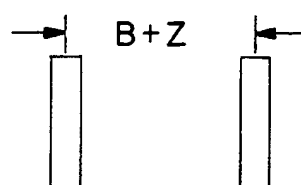


FIG. 26




FIG. 27




FIG. 28

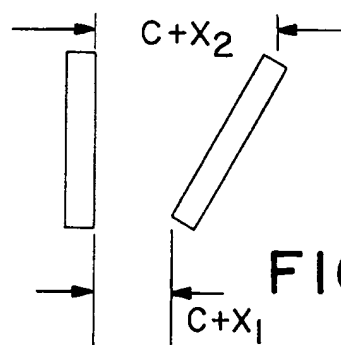


FIG. 29

SUBSTITUTE SHEET (RULE26)

17/ 23

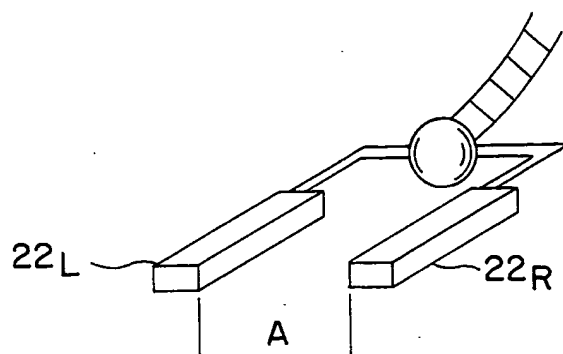


FIG. 30

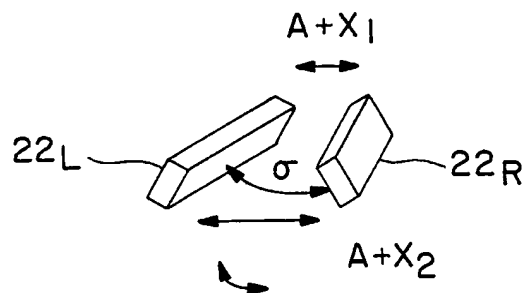


FIG. 31

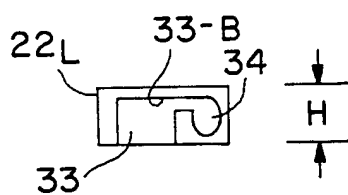


FIG. 32

18/23

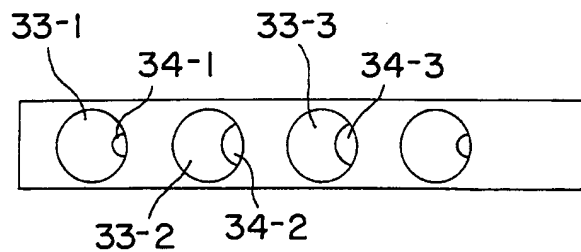


FIG. 33

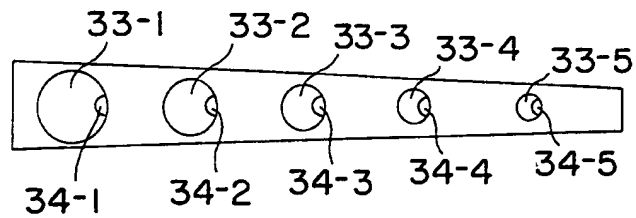


FIG. 34

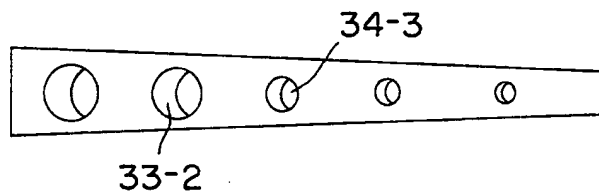


FIG. 35

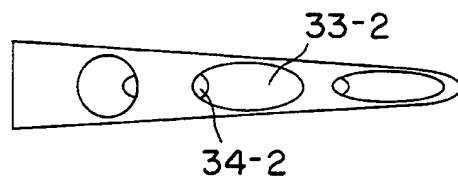


FIG. 36

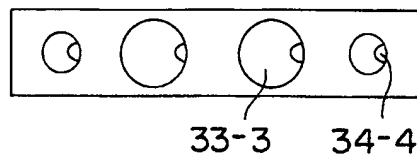


FIG. 37

19 / 23

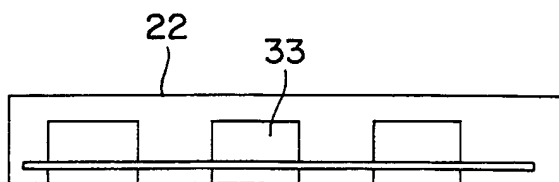


FIG. 38

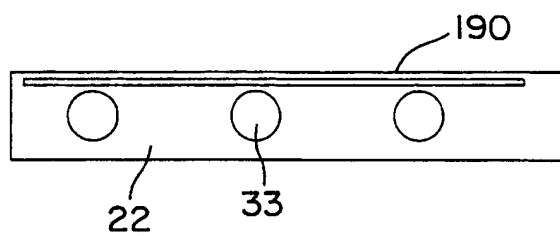


FIG. 39

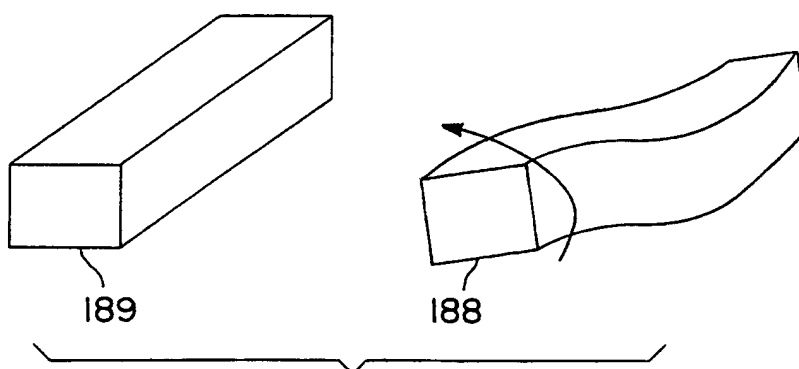


FIG. 40

20/23

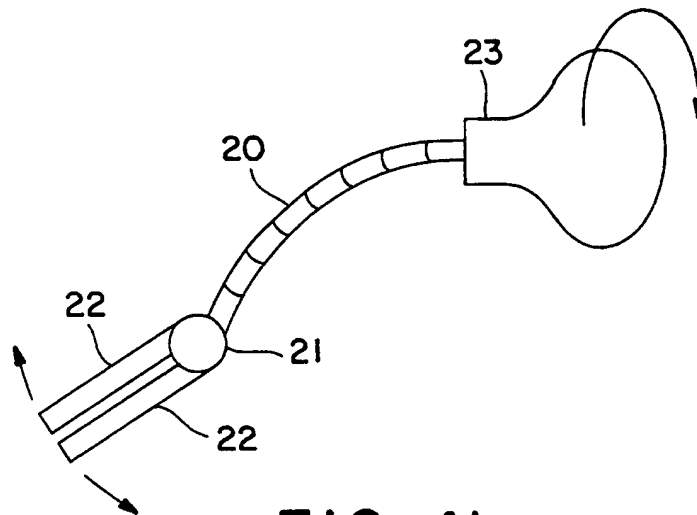


FIG. 41

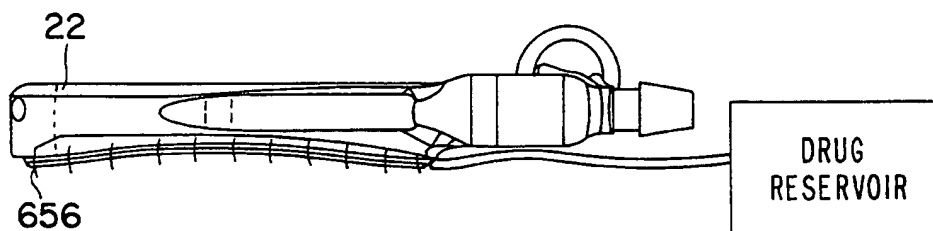


FIG. 42

21/23

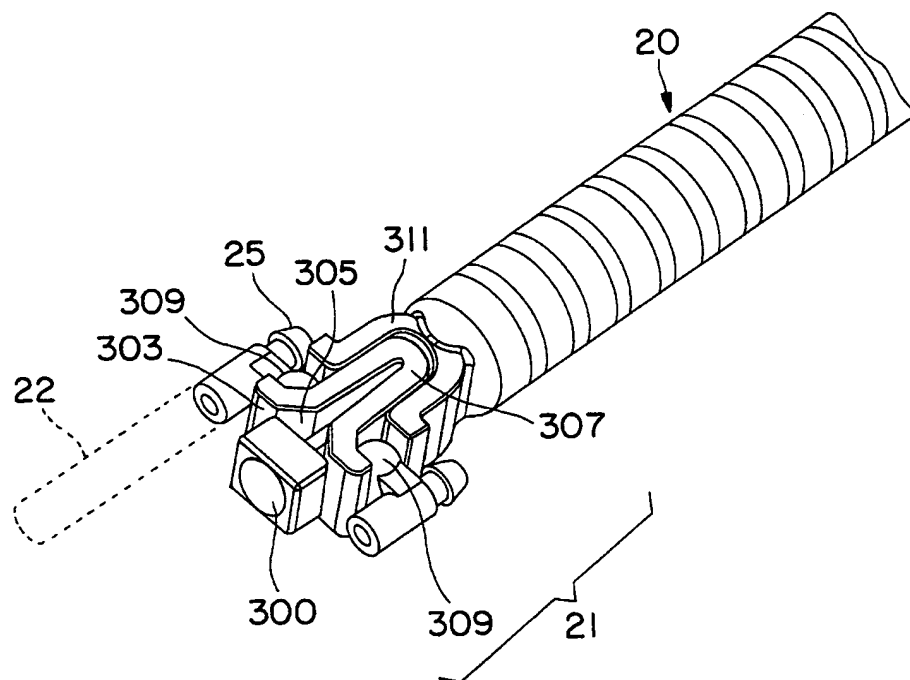


FIG. 43

22/ 23

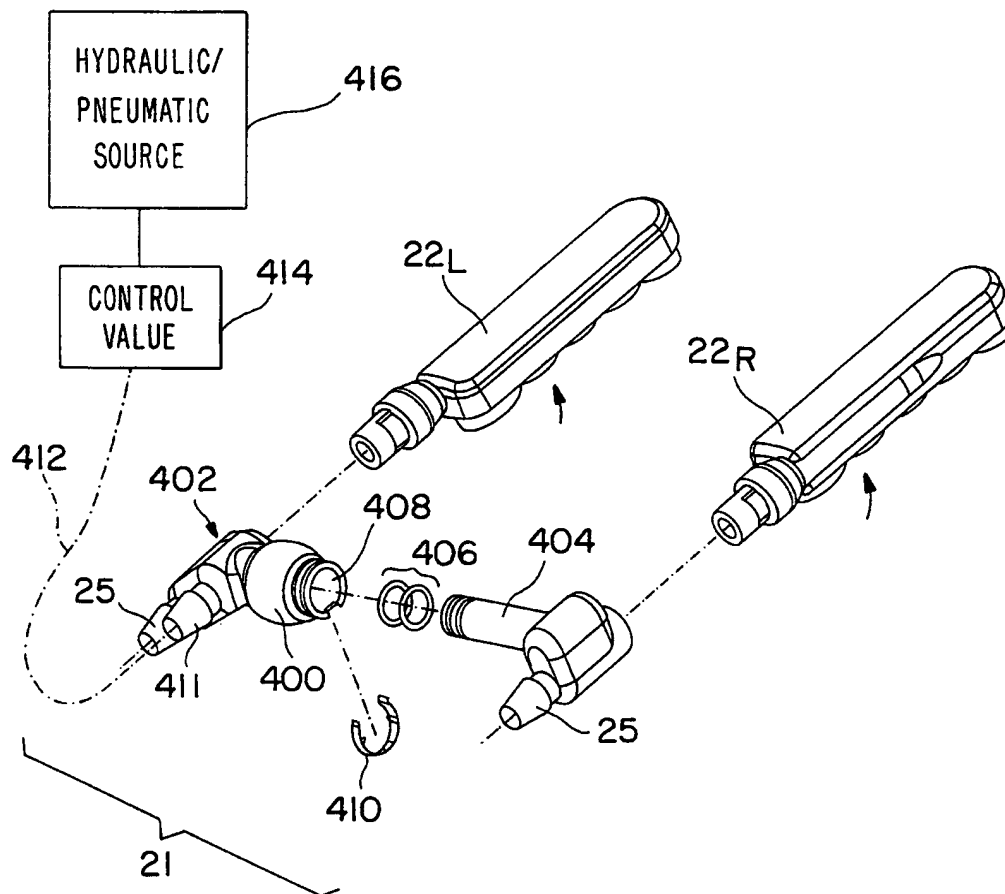


FIG. 44

23 / 23

